



V4.55.64  
29/09/2026

# SASstudio4 User Guide

# Content

|                                                                                                                               |          |
|-------------------------------------------------------------------------------------------------------------------------------|----------|
| <b>1. Version Management.....</b>                                                                                             | <b>1</b> |
| <b>2. Preface .....</b>                                                                                                       | <b>3</b> |
| <b>3. Preparation .....</b>                                                                                                   | <b>4</b> |
| 3.1 Software Compatibility .....                                                                                              | 4        |
| 3.2 Operating Environment Requirements .....                                                                                  | 4        |
| 3.3 Default Software Storage Paths .....                                                                                      | 4        |
| 3.4 Software Acquisition.....                                                                                                 | 5        |
| <b>4. Working Modes Overview .....</b>                                                                                        | <b>6</b> |
| 4.1 Standard Spectrum Analysis .....                                                                                          | 6        |
| 4.2 Receiver/IQ Streaming Mode .....                                                                                          | 6        |
| 4.3 Power Detection Mode .....                                                                                                | 6        |
| 4.4 Real-Time Spectrum Analysis Mode .....                                                                                    | 7        |
| 4.5 Harmonic Analysis Mode .....                                                                                              | 7        |
| 4.6 Phase Noise Measurement Mode.....                                                                                         | 7        |
| 4.7 Digital Demodulation Mode (Option 71).....                                                                                | 7        |
| 4.8 Application Software UI Layout .....                                                                                      | 7        |
| 4.8.1 Menu .....                                                                                                              | 8        |
| 4.8.2 Graph Set Area.....                                                                                                     | 8        |
| 4.8.3 Main Settings Area .....                                                                                                | 8        |
| 4.8.4 Instrument State .....                                                                                                  | 8        |
| <b>5. Common Operation .....</b>                                                                                              | <b>9</b> |
| 5.1 Save and Recall Instrument Configuration .....                                                                            | 9        |
| 5.2 Save the Pictures .....                                                                                                   | 9        |
| 5.3 Deleting files and images .....                                                                                           | 9        |
| 5.4 Setting the Startup State.....                                                                                            | 9        |
| 5.5 Switching Operating Modes.....                                                                                            | 10       |
| 5.6 Professional and Concise Settings .....                                                                                   | 10       |
| 5.7 Theme Settings .....                                                                                                      | 10       |
| 5.8 Parameter Settings.....                                                                                                   | 10       |
| 5.9 GNSS Usage .....                                                                                                          | 11       |
| 5.9.1 Using the internal GNSS Source.....                                                                                     | 12       |
| 5.9.2 Using the External EIO GNSS Module .....                                                                                | 12       |
| 5.9.3 Using the External USB GNSS Module .....                                                                                | 13       |
| 5.9.4 1PPS Trigger Using Default GNSS Source .....                                                                            | 14       |
| 5.9.5 Using the 10 MHz Reference Clock of the external EIO GNSS Module<br>(Available Only on High-Quality GNSS Modules) ..... | 14       |
| 5.9.6 Reference Clock Calibration .....                                                                                       | 15       |
| 5.10 GPIO Output Level Control .....                                                                                          | 16       |

|         |                                        |    |
|---------|----------------------------------------|----|
| 5.11    | Viewing Instrument Information.....    | 16 |
| 5.12    | Preset .....                           | 16 |
| 5.13    | Single or Continuous Preview .....     | 16 |
| 5.14    | Quick Record and Playback .....        | 16 |
| 5.15    | Hide Panel .....                       | 16 |
| 5.16    | Y-Axis Scale Zoom .....                | 17 |
| 5.17    | Offset .....                           | 17 |
| 5.18    | Switch X-Axis scale.....               | 17 |
| 5.19    | Display Line .....                     | 17 |
| 5.20    | Setting Chart Units .....              | 17 |
| 5.21    | Spectrogram .....                      | 17 |
| 5.22    | Export Data .....                      | 18 |
| 5.23    | Record and Playback .....              | 18 |
| 5.24    | Graph Zoom Function.....               | 19 |
| 5.24.1  | Zoom Function.....                     | 19 |
| 5.24.2  | Magnifying Glass Function .....        | 20 |
| 5.24.3  | Interactive Zoom(PX series only) ..... | 21 |
| 5.25    | Trace settings.....                    | 21 |
| 5.26    | Marker Function .....                  | 22 |
| 5.26.1  | Create Markers.....                    | 22 |
| 5.26.2  | Create Marker Pairs.....               | 22 |
| 5.26.3  | Close Markers.....                     | 22 |
| 5.26.4  | Change Markers Frequency .....         | 22 |
| 5.26.5  | Marker switching traces .....          | 22 |
| 5.26.6  | Delta Marker .....                     | 23 |
| 5.26.7  | Noise Density .....                    | 23 |
| 5.26.8  | Marker Peak Search .....               | 23 |
| 5.26.9  | Marker to Center.....                  | 24 |
| 5.26.10 | Marker Switch to Mode.....             | 24 |
| 5.26.11 | Signal tracking .....                  | 24 |
| 5.26.12 | Peak tracking .....                    | 25 |
| 5.26.13 | Peak table .....                       | 25 |
| 5.27    | Quick Parameter Setting .....          | 26 |
| 5.27.1  | Parameter setting.....                 | 26 |
| 5.27.2  | Parameter display.....                 | 27 |
| 5.28    | Modifying the IQSampleRate .....       | 27 |
| 5.29    | Amplitude Correction .....             | 27 |
| 5.29.1  | Correction Rules .....                 | 27 |
| 5.29.2  | Amplitude Correction Example .....     | 27 |
| 5.30    | Antenna Attitude .....                 | 28 |
| 5.30.1  | Interface Description.....             | 28 |
| 5.30.2  | Parameter Description .....            | 29 |
| 5.30.3  | Steps for Using with HDA-series.....   | 30 |

|           |                                                             |           |
|-----------|-------------------------------------------------------------|-----------|
| 5.31      | Display modes (only in SA/NX series) .....                  | 30        |
| 5.32      | SCPI Remote Control .....                                   | 31        |
| <b>6.</b> | <b>Using of the SWP mode .....</b>                          | <b>32</b> |
| 6.1       | Introduction to the General Parameters of the SWP Mode..... | 32        |
| 6.2       | Channel Power.....                                          | 34        |
| 6.2.1     | Parameters description .....                                | 34        |
| 6.2.2     | Procedure .....                                             | 34        |
| 6.3       | Occupied Bandwidth.....                                     | 35        |
| 6.3.1     | Parameters description .....                                | 35        |
| 6.3.2     | Procedure .....                                             | 35        |
| 6.4       | Adjacent Channel Power Ratio (ACPR).....                    | 36        |
| 6.4.1     | Parameters description .....                                | 36        |
| 6.4.2     | Procedure .....                                             | 36        |
| 6.5       | IP3/IM3.....                                                | 37        |
| 6.5.1     | Parameters description .....                                | 37        |
| 6.5.2     | Procedure .....                                             | 37        |
| 6.6       | SEM.....                                                    | 38        |
| 6.6.1     | Parameters description .....                                | 38        |
| 6.6.2     | Procedure .....                                             | 39        |
| 6.7       | Auto Reference Level.....                                   | 39        |
| 6.8       | Antenna Factor .....                                        | 40        |
| 6.8.1     | Parameters description .....                                | 40        |
| 6.8.2     | Compensation Rules .....                                    | 40        |
| 6.8.3     | Antenna Factor Configuration Example.....                   | 41        |
| 6.8.4     | Auto Load Antenna Factor .....                              | 41        |
| <b>7.</b> | <b>Using of the IQS mode .....</b>                          | <b>43</b> |
| 7.1       | Introduction to the General Parameters of The IQS mode..... | 43        |
| 7.2       | IQ Streaming Working Mode Overview .....                    | 44        |
| 7.3       | Spectrum Analysis.....                                      | 44        |
| 7.3.1     | Parameters description .....                                | 44        |
| 7.3.2     | Procedure .....                                             | 44        |
| 7.4       | IQvT.....                                                   | 45        |
| 7.4.1     | Procedure .....                                             | 45        |
| 7.5       | PvT .....                                                   | 46        |
| 7.5.1     | Procedure .....                                             | 46        |
| 7.6       | AM Demodulation .....                                       | 46        |
| 7.6.1     | Parameters description .....                                | 46        |
| 7.6.2     | Procedure .....                                             | 47        |
| 7.6.3     | Audio analysis.....                                         | 47        |
| 7.7       | FM Demodulation.....                                        | 48        |
| 7.7.1     | Parameters description .....                                | 48        |

|            |                                                                   |           |
|------------|-------------------------------------------------------------------|-----------|
| 7.7.2      | Procedure .....                                                   | 48        |
| 7.7.3      | Audio analysis.....                                               | 49        |
| 7.8        | DDC Digital Down Conversion .....                                 | 49        |
| 7.8.1      | Parameters description .....                                      | 49        |
| 7.8.2      | Procedure .....                                                   | 49        |
| <b>8.</b>  | <b>Using of the DET Mode .....</b>                                | <b>51</b> |
| 8.1        | Introduction to the General Parameters of DET Mode .....          | 51        |
| 8.2        | Pulse Signal Measurement .....                                    | 51        |
| 8.2.1      | Procedure .....                                                   | 51        |
| 8.3        | Pulse Signal Detection (Option 72) .....                          | 52        |
| 8.3.1      | Parameters description .....                                      | 52        |
| 8.3.2      | Procedure .....                                                   | 52        |
| <b>9.</b>  | <b>Using of the RTA mode.....</b>                                 | <b>54</b> |
| 9.1        | Introduction to the General Parameters of RTA Mode .....          | 54        |
| 9.2        | Probability Density Plot .....                                    | 55        |
| 9.2.1      | Parameters description .....                                      | 55        |
| 9.2.2      | Density Display Range.....                                        | 55        |
| 9.2.3      | Persistence Settings.....                                         | 55        |
| 9.2.4      | Close Probability Density Plot.....                               | 55        |
| 9.3        | WIFI Signal Measurement .....                                     | 56        |
| <b>10.</b> | <b>Digital Demodulation (Option 71) .....</b>                     | <b>58</b> |
| 10.1       | Parameters description .....                                      | 58        |
| 10.2       | Function Overview.....                                            | 58        |
| 10.3       | Procedure.....                                                    | 58        |
| <b>11.</b> | <b>Harmonic Analysis Mode.....</b>                                | <b>60</b> |
| 11.1       | Version Requirements.....                                         | 60        |
| 11.2       | Enable Harmonic Analysis Function .....                           | 60        |
| 11.3       | Parameters description .....                                      | 60        |
| 11.4       | Procedure.....                                                    | 61        |
| <b>12.</b> | <b>Phase Noise Measurement Mode.....</b>                          | <b>62</b> |
| 12.1       | Version Requirements.....                                         | 62        |
| 12.2       | Enable Phase Noise Measurement Function .....                     | 62        |
| 12.3       | Parameters description .....                                      | 62        |
| 12.4       | Procedure.....                                                    | 63        |
| 12.4.1     | Phase Noise Measurement with Known Carrier Information .....      | 63        |
| 12.4.2     | Phase Noise Measurement with Unknown Carrier Information .....    | 64        |
| <b>13.</b> | <b>Signal/Tracking Generator Function (Option 60 61 62) .....</b> | <b>65</b> |
| 13.1       | Instructions for Using the ASG Function .....                     | 66        |
| 13.1.1     | Output a Single-Tone Signal .....                                 | 66        |

|            |                                                                    |           |
|------------|--------------------------------------------------------------------|-----------|
| 13.1.2     | Output a Frequency Sweep Signal.....                               | 66        |
| 13.1.3     | Output a Power Sweep Sigal .....                                   | 67        |
| 13.1.4     | Tracking Generator (TG).....                                       | 67        |
| <b>14.</b> | <b>EMI Pre-Compliance Measurements (Option 74).....</b>            | <b>69</b> |
| 14.1       | Version Requirements .....                                         | 69        |
| 14.2       | Introduction to EMI Pre-Compliance Measurements .....              | 69        |
| 14.3       | Introduction to EMI Pre-Compliance Mode Interface .....            | 69        |
| 14.4       | Introduction to General Parameters for EMI Pre-Compliance .....    | 71        |
| 14.5       | Operating Steps .....                                              | 72        |
| <b>15.</b> | <b>Additional Functions .....</b>                                  | <b>74</b> |
| 15.1       | Description of Trigger Functions .....                             | 74        |
| 15.1.1     | SWP Frequency Sweep Mode .....                                     | 74        |
| 15.1.2     | Fixed Frequency Point Mode for IQS, DET and RTA .....              | 74        |
| 15.2       | IF Output Application Guide .....                                  | 75        |
| 15.3       | External Reference Clock Input .....                               | 75        |
| 15.4       | Connecting and Operating Multiple Instruments Simultaneously ..... | 76        |
| <b>16.</b> | <b>Application for Options .....</b>                               | <b>77</b> |
| 16.1       | Pulse Detection Option .....                                       | 77        |
| 16.1.1     | Application for License .....                                      | 77        |
| 16.1.2     | License Placement .....                                            | 77        |
| 16.2       | Digital Demodulation Option.....                                   | 78        |
| 16.2.1     | Application for License and Digital Demodulation Library .....     | 78        |
| 16.2.2     | License and Digital Demodulation Library Placement.....            | 78        |
| 16.3       | AUXS Option.....                                                   | 78        |
| 16.4       | EMI Pre-Compliance Measurements Option .....                       | 78        |
| 16.4.1     | Apply for a License .....                                          | 78        |
| 16.4.2     | Place the License.....                                             | 78        |
| <b>17.</b> | <b>Software and Firmware Update .....</b>                          | <b>79</b> |
| 17.1       | Version Requirements.....                                          | 79        |
| 17.2       | Parameter Description .....                                        | 79        |
| 17.3       | Online Download .....                                              | 79        |
| 17.4       | Import Offline Package .....                                       | 80        |
|            | <b>Appendix .....</b>                                              | <b>82</b> |
|            | <b>Appendix 1: Record File Format Description .....</b>            | <b>82</b> |
| 1.1        | File Naming Format.....                                            | 82        |
| 1.2        | Conversion of Structures into Byte Arrays .....                    | 82        |
|            | <b>Appendix 2: Standard Spectrum Analysis Mode.....</b>            | <b>83</b> |
|            | <b>Appendix 3: Receiver/IQ Stream Mode .....</b>                   | <b>87</b> |

|                                                    |    |
|----------------------------------------------------|----|
| Appendix 4: Power Detection Mode .....             | 92 |
| Appendix 5: Real-Time Spectrum Analysis Mode ..... | 97 |

# 1. Version Management

## Updated Description Sheet

| Version    | Description                                                                                                                                                                                                                                                                                                                                                | Date       |
|------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|------------|
| V4.55.64   | 1. Modified: <a href="#">SCPI Remote Control</a> chapter<br>2. Modified: <a href="#">Using of the RTA mode</a> chapter                                                                                                                                                                                                                                     | 29/09/2026 |
| V4.55.52   | 1. Added: <a href="#">SCPI Remote Control</a> chapter<br>2. Modified: <a href="#">EMI Pre-Compliance Measurements (Option 74)</a> chapter                                                                                                                                                                                                                  | 20/08/2026 |
| V4.55.50   | 3. Modified: <a href="#">GNSS usage</a> chapter<br>4. Modified: <a href="#">Software and Firmware Update</a> chapter<br>5. Added: <a href="#">EMC (Option 74)</a> chapter<br>6. Added: <a href="#">EMC Option</a> section in the <a href="#">Application for Options</a> chapter                                                                           | 29/07/2026 |
| V4.55.48   | 7. Added: <a href="#">AGC Period</a> parameter description<br>8. Modified: Mapping Mode chapter                                                                                                                                                                                                                                                            | 14/07/2026 |
| V4.55.44   | 1. Added: <a href="#">Antenna Attitude</a> chapter                                                                                                                                                                                                                                                                                                         | 02/07/2026 |
| V4.55.43   | 1. Added: A new section on <a href="#">Custom Image Map Mode</a> has been added to the Heatmap Mode chapter<br>2. Modified: The GNSS source configuration strategy in the <a href="#">GNSS usage</a> section has been reorganized                                                                                                                          | 19/05/2026 |
| V4.55.41   | 1. Added: <a href="#">TG</a> chapter<br>2. Added: MSCAN chapter<br>3. Added: <a href="#">Fan control</a> description added in Parameter Setting section<br>4. Modified: <a href="#">Software and Firmware Update</a> chapter                                                                                                                               | 13/04/2026 |
| V3.55.32.0 | 1. Added: Mapping mode chapter                                                                                                                                                                                                                                                                                                                             | 03/02/2026 |
| V3.55.30.1 | 1. Modified: Updated the <a href="#">License Placement section</a> for the Pulse Detection Option<br>2. Modified: Updated the <a href="#">License and Digital Demodulation Library Placement</a> section for the Digital Demodulation Option<br>3. Modified: Updated the <a href="#">Firmware Update for PX Series Instrument on Linux Systems</a> section | 20/11/2025 |
| V3.55.30.0 | 1. Added: <a href="#">Spectrum Color Bar power range adjustment method</a> in Spectrogram chapter<br>2. Updated: Optimized version management<br>3. Added: <a href="#">Record File Format Description</a>                                                                                                                                                  | 07/11/2025 |
| V3.55.29.0 | 1. Updated: Document version number (no content changes)                                                                                                                                                                                                                                                                                                   | 24/10/2025 |

|      |                                                                                                |            |
|------|------------------------------------------------------------------------------------------------|------------|
| V1.3 | 1. Added: <a href="#">Auto Reference Level</a> chapter                                         | 20/10/2025 |
|      | 2. Added: <a href="#">Auto Load Antenna Factor</a> chapter                                     |            |
|      | 3. Added: <a href="#">Average Number parameter description</a> in Digital Demodulation Mode    |            |
|      | 4. Modified: <a href="#">AM/FM</a> Demodulation operation instructions                         |            |
| V1.2 | 1. Modified: <a href="#">AM/FM</a> Demodulation chapters based on new functionality            | 08/09/2025 |
|      | 2. Modified: <a href="#">Software Update for PX Series Instrument</a> chapter                  |            |
|      | 3. Added: <a href="#">Firmware update for PX Series Instrument on Linux system</a> chapter     |            |
|      | 4. Added: <a href="#">Connecting and Operating Multiple Instruments Simultaneously</a> chapter |            |
|      | 5. Added: <a href="#">Antenna Factor</a> chapter                                               |            |
|      | 6. Added: <a href="#">Y-Axis Scale Zoom</a> chapter                                            |            |
|      | 7. Added: <a href="#">Interactive zoom (PX series only)</a> in Graph Zoom Function chapter     |            |
|      | 8. Added: <a href="#">Center Frequency and Span setting</a> in Quick Parameter Setting chapter |            |
| V1.1 | 1. Added: <a href="#">Switch X-Axis Scale</a> chapter                                          | 25/08/2025 |
|      | 2. Added: <a href="#">Peak Tracking</a> chapter                                                |            |
|      | 3. Added: <a href="#">Auto parameter setting</a> in Left/Right Peak Search                     |            |
| V1.0 | 1. Initial Version                                                                             | 08/08/2025 |

# 2. Preface

The software supports three display modes:

- **SA/NX Series instruments and R Series RF Receivers:** workstation one column (default), workstation two column, and tablet mode
- **PX Series instruments:** Tablet mode

This document uses the tablet mode in the software as an example to describe the interface layout, operating modes, and operation methods of the SASudio4 software. Although the supported display modes vary among different instruments, the operation logic is consistent across all modes. The corresponding interface diagrams are shown below.

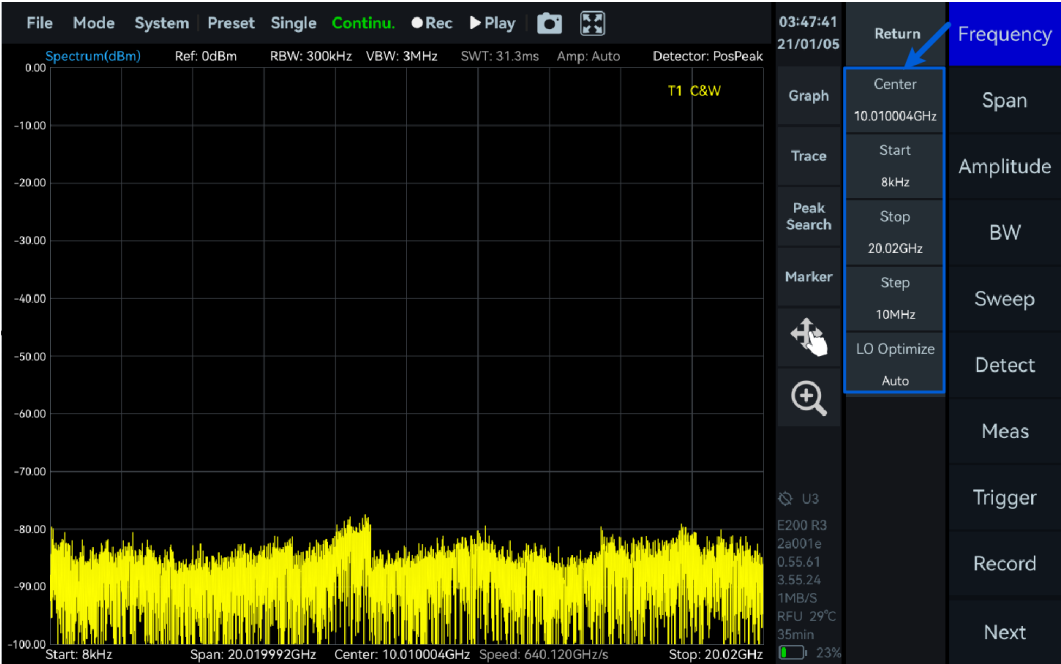


Figure 1 Tablet mode interface display

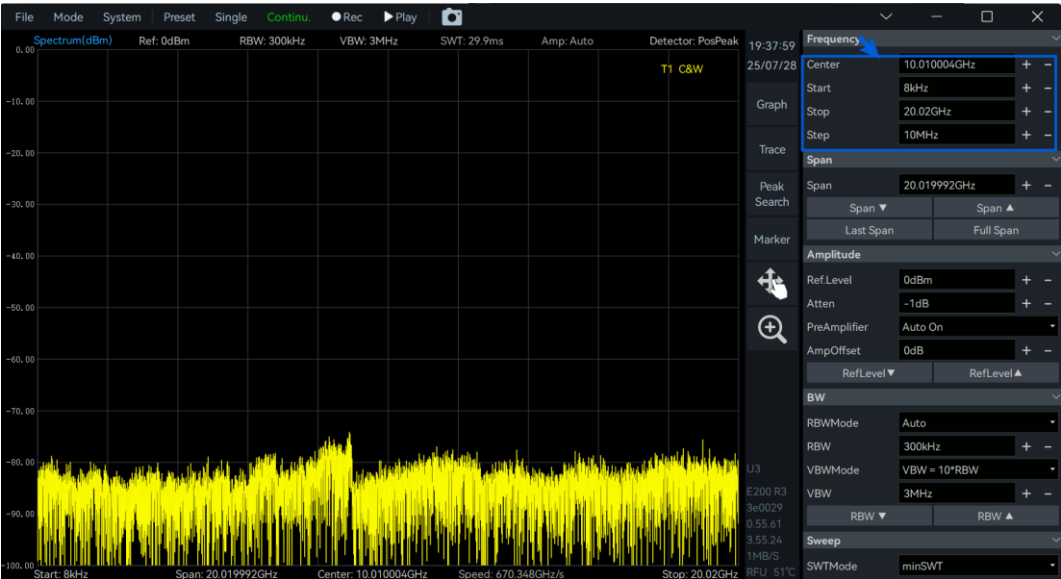


Figure 2 Workstation one column mode interface display

## 3. Preparation

### 3.1 Software Compatibility

SASstudio4 supports all SA, NX, and PX Series instruments with version 55, as well as R Series RF receivers. For information on using R Series RF receivers, refer first to the *R1000 Series RF Receiver User Manual*. For operations of R Series products described in this *SASstudio4 User Guide*, refer to the instructions for the SA/NX Series.

### 3.2 Operating Environment Requirements

For the SA/NX series, which are kernel-based instruments, the SASstudio4 software must be installed on a host computer. The recommended operating environment for the host computer is shown in the table below:

Only the basic recommended configurations are listed in the table. For systems below the recommended specifications, please refer to the actual test results.

**Table 1 System Operating Environment Requirements**

|                           |                                                                                                                                        |
|---------------------------|----------------------------------------------------------------------------------------------------------------------------------------|
| <b>Operating System</b>   | Windows 11/10/8/7, requires VS2019 C++ redistributables<br><br>Ubuntu 22.04/20.04/18.04, Debian 12/11/10, Raspberry Pi OS 64-bit       |
| <b>Architecture</b>       | Windows: x64, AArch64 (only on NX devices)<br><br>Linux: x64, AArch64                                                                  |
| <b>Processor</b>          | Windows: Intel i3 or above; AArch64 (tested on 8CX Gen2)<br><br>Linux: Tested on Raspberry Pi 4B, Raspberry Pi 5, RK3399, RK3588, etc. |
| <b>Memory</b>             | 4 GB or above                                                                                                                          |
| <b>Storage</b>            | IQ recording requires sustained storage write speed >400 Mbytes/s                                                                      |
| <b>Data Interface</b>     | USB 2.0 or USB 3.0 (USB 3.0 recommended), or 1GbE Ethernet<br><br>IQ recording bandwidth and duration depend on interface bandwidth    |
| <b>Display Resolution</b> | Not less than 1280 * 800 pixels                                                                                                        |
| <b>Other</b>              | Certain antivirus software may cause the system to malfunction                                                                         |

### 3.3 Default Software Storage Paths

**PXE-90/PXE-200/PXN-400 Series Instruments:** The software is installed in the userdata directory on the desktop by default;

**PXN-45/PXN-60/PXN-90 Series Instruments and the Embedded Hosts of R Series RF Receivers:** The software is installed in the /software directory by default;

**SA/NX Series Instruments and Host Computers for R Series RF Receivers:** User-defined directory.

In the software directory, the "data", "images", and "reports" folders store different types of data respectively.

- **data folder:** Recording files, Configuration files, and Spectrogram CSV data files
- **images folder:** Chart images
- **reports folder:** CSV files containing chart data and the corresponding configuration files

Except for [quick record/playback](#) files and [quick screenshots](#), all other recording files or images can be stored in a user-defined path (PX series instruments require an external storage device, while SA/NX series instruments can define the storage path directly).

### 3.4 Software Acquisition

Please refer to the [Software and Firmware Update](#) section for instructions on obtaining and installing the latest version of the software.

Note: By default, Windows x64, Linux x86\_64 and Linux aarch64 versions of the software are provided. If a Windows x86 version is required, please contact official technical support for assistance.

## 4. Working Modes Overview

Software offers working modes, including Standard Spectrum Analysis (SWP), IQ Streaming (IQS), Power Detection Analysis (DET), Real-time Spectrum Analysis (RTA), Phase Noise Measure, Basic Digital Demodulation (option), Harmonic Analysis, and EMI Pre-Compliance (option). The measurement functions available in each working mode will be explained in the following sections.

### 4.1 Standard Spectrum Analysis

In the standard spectrum analysis mode, the instrument performs frequency hopping according to the configuration to achieve frequency scanning. This mode is suitable for applications focused on frequency trace measurement and analysis. The measurement and analysis functions provided in the standard spectrum analysis mode include:

- Spectrum Panoramic Sweep
- Local Spectrum Zoom Display
- Spectrogram
- Spectrum Recording and Playback
- SEM
- Peak and Signal Tracking
- IM3
- Channel Power
- OBW
- ACPR
- Amplitude Correction
- Peak Table

### 4.2 Receiver/IQ Streaming Mode

In the IQ streaming mode, the instrument acquires time-domain data within the analysis bandwidth according to the specified trigger signal and returns it to the user. This mode is suitable for applications such as time-domain signal recording and basic demodulation analysis. The functions provided in the IQ streaming mode include:

- IQ Time Domain Waveform
- Spectrogram
- Power-Time Waveform
- Multi-Channel DDC
- Pulse Signal Detection (option)
- Spectrum Analysis
- AM/FM Demodulation
- Audio Analysis
- IQ Data Recording and Playback

### 4.3 Power Detection Mode

In the detector analysis mode, the instrument performs continuous detection analysis on the time-domain signal within the analysis bandwidth. This mode is suitable for observing the relationship between time and power within a certain bandwidth, such as pulse parameter measurements. The functions provided in the detector analysis mode include:

- Power-Time waveform and zoom
- Pulse Signal Detection (option)
- DET Data Recording and Playback

#### 4.4 Real-Time Spectrum Analysis Mode

In the real-time spectrum analysis mode, the instrument performs real-time spectrum analysis on the time-domain signal within the analysis bandwidth and returns the spectrum results to the user. This mode is suitable for applications that focus on instantaneous and transient signals, such as interference troubleshooting and the identification of characteristic signals in complex electromagnetic environments. The functions provided in the real-time spectrum analysis mode include:

- Real-time Spectrum Probability
- Real-Time Spectrum Data Recording and Density Graph and Spectrogram
- Playback

#### 4.5 Harmonic Analysis Mode

In the harmonic analysis mode, the instrument performs harmonic analysis on the signal based on its fundamental frequency and displays the frequency, amplitude, and the relative difference from the fundamental for each harmonic. This mode is suitable for analyzing harmonic distortion in signals and helps identify and evaluate their nonlinear characteristics. The functions provided in the harmonic analysis mode include:

- Harmonic Spectrum Diagram
- Harmonic Measurement Table

#### 4.6 Phase Noise Measurement Mode

In the phase noise measurement mode, the instrument uses automated measurement techniques to provide high-precision phase noise plots and detailed data tables, enabling users to thoroughly analyze the phase stability of a signal and the noise density at different frequency offsets. The functions provided in the phase noise measurement mode include:

- SSB Phase Noise Spectrum Diagram
- Phase Noise Measurement Table

#### 4.7 Digital Demodulation Mode (Option 71)

In the digital demodulation mode, the instrument supports demodulation of various modulated signals and evaluates their modulation quality from multiple perspectives. This function is suitable for a wide range of applications, particularly for in-depth analysis and quality assessment of known modulated signals. The functions provided in the digital demodulation mode include:

- Constellation and Eye Diagram
- Bit Table and Demodulation
- Modulated Signal Spectrum Analysis
- ASK/FSK/PSK/QAM Demodulation

#### 4.8 Application Software UI Layout

The application software UI consists of the following sections:

- Menu
- Graph Set Area
- Graph Display Area
- Main Setting Area
- Instrument State
- Parameter Quick Set

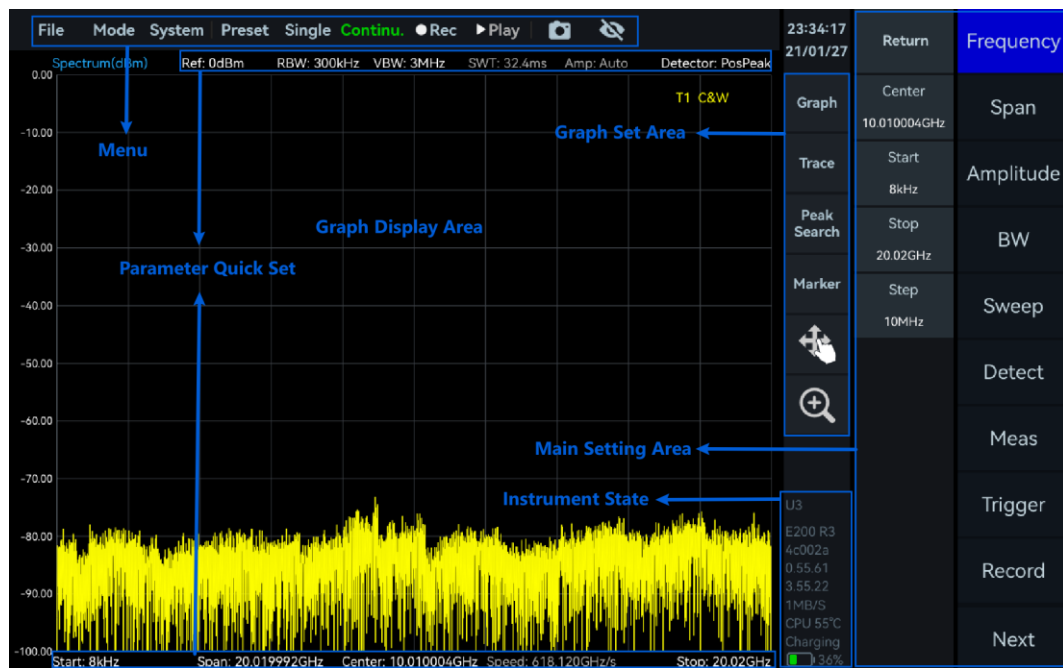


Figure 3 Software Interface Layout

#### 4.8.1 Menu

- Save and Load Configuration
- Working Mode Switch
- Single or Continuous Preview
- Quick Screenshot
- Fan Control (SA/NX only)
- Set Startup State
- Measurement Mode Selection
- Recording and Playback
- GNSS and Instrument Information View
- Display Mode Switch (SA/NX only)

#### 4.8.2 Graph Set Area

- Graph Settings
- Marker Settings
- Trace Settings
- Display Measurement Results

#### 4.8.3 Main Settings Area

- Measurement and Analysis Settings
- Data Recording and Playback
- Trigger Settings
- System Settings

#### 4.8.4 Instrument State

- GNSS Antenna Connections Status
- Last Six Digits of Instrument UID
- Software GUI Version
- Instrument Real-Time Temperature
- Instrument Model
- API/FPGA/MCU Version
- Bus Data Throughput
- Instrument Power Level (PX only)

## 5. Common Operation

### 5.1 Save and Recall Instrument Configuration

1. Save the current configuration
  - 1). Click "File" -> "Save State" in the menu bar;
  - 2). In the "Save Configuration File" pop-up window, set the save path and file name, click "Confirm" to save the configuration file.
2. Open pre-stored configurations
  - 1). Click "File" -> "Recall State" in the menu bar;
  - 2). Select the configuration file in the "Please select file" pop-up window, click "Confirm" to open the pre-stored configuration.

### 5.2 Save the Pictures

1. Click "File" -> "Save Image" on the menu bar;
2. In the "Save Image" pop-up window, set the path to save the picture and the picture name, and click "Confirm" to save the screenshot.
3. Users can also take screenshots by clicking the shortcut button  in the menu bar, the pictures are saved in the `/images` folder by default, and the storage path cannot be changed.

### 5.3 Deleting files and images

**PXE-90/PXE-200/PXN-400 Series Instruments:** In the corresponding [storage folder](#) under the software directory, drag and drop the target file to the "Trash Can", then click "Yes" in the confirmation dialog to delete it. (The deletion method for record files and configuration files is the same as for screenshots).

**PXN-45/PXN-60/PXN-90 Series Instruments:** In the corresponding [storage folder](#) under the software directory, select the target file, then click "Edit" -> "Move to Trash" in the top menu bar. Finally, click "Yes" in the confirmation dialog to complete the deletion.

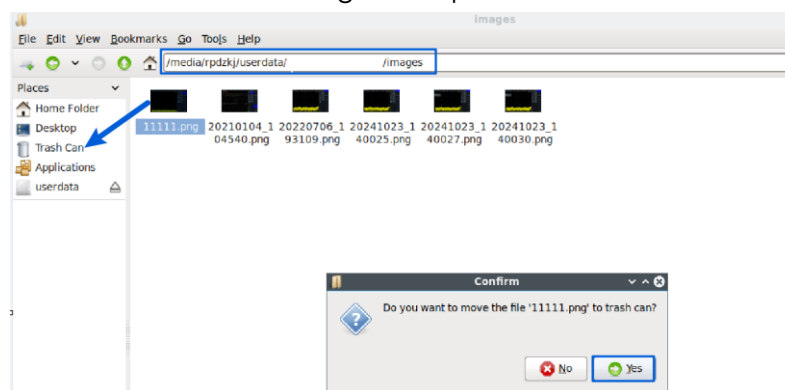


Figure 4 PXE-90/PXE-200/PXN-400 Series Instruments Delete Picture

### 5.4 Setting the Startup State

The instrument supports user-defined startup states, the relevant startup state description is detailed in Table below.

**Table 2 Upper computer software power on state**

| No. | Power On State |                                                         |
|-----|----------------|---------------------------------------------------------|
| 1   | Default        | Default configuration.                                  |
| 2   | User Preset    | Load a user-saved profile as the startup configuration. |
| 3   | Last State     | Restore settings from the last session at startup.      |

If you want to set the startup state, follow these steps.

1. Click "File" -> "Power On State" in the menu bar;
2. "Default" and "Last State" can be ticked directly, the software will take this option as the initial state when it starts next time;
3. Select "User Preset", select the user's pre-saved configuration file in the "Please select file" pop-up window that appears, and the software will open with the specified configuration at the next startup.

### 5.5 Switching Operating Modes

Click "Mode" in the menu bar to switch between Standard Spectrum Analysis, Receiver/IQ Streaming, Power Detection, Real-Time Spectrum Analysis, Digital Demodulation (Option), Harmonic Analysis, Phase Noise Measurement, and EMI Pre-Compliance (Option).

### 5.6 Professional and Concise Settings

Click "System" -> "Setting Mode" in the menu bar to switch between "Basic" and "Professional" modes. Compared to the Basic mode, the Professional mode provides more parameter options in the main settings area, allowing users to flexibly select the appropriate setting mode based on actual needs.

### 5.7 Theme Settings

Click "System" -> "Theme" in the menu bar to switch between "Dark" and "Light" themes.

### 5.8 Parameter Settings

Click "System" -> "Preference" in the menu bar, and you can set the following functions in the pop-up setting window:

**Table 3 Parameter Setting Parameter Description**

| Parameter            | Description                                                                                                                                                                             |
|----------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Haptics (PX only)    | When enabled, the instrument provides haptic feedback via vibration during touchscreen operations.                                                                                      |
| Screen Lock          | When enabled, a lock icon "🔒" appears on the right side of the screen. Tap the icon "🔒" to lock the screen and prevent accidental operations, tap again to unlock.                      |
| Digital Det          | When enabled, reduces the refresh rate of certain displayed parameters (including marker) to aid observation and recording.                                                             |
| Auto-Dim (PX only)   | When enabled, the instrument automatically lowers screen brightness if there is no operation for one minute.                                                                            |
| Brightness (PX only) | Adjusts the screen brightness for PX series instruments.                                                                                                                                |
| Volume (PX only)     | Adjusts the volume for PX series instruments.                                                                                                                                           |
| Date/Time (PX only)  | When GNSS is not locked, the user can manually set the PX series system time. Once GNSS is locked, system time can be synchronized either by a one-time "Auto UTC Time" or continuously |

via "Sync UTC Time".

|                       |                                                         |
|-----------------------|---------------------------------------------------------|
| Fan Control (PX only) | Standard: lower temperature threshold, more responsive. |
|                       | Quiet: higher threshold, smoother speed ramp.           |

## 5.9 GNSS Usage

This section provides detailed instructions on how to acquire real-time positioning data using the internal GNSS, external EIO GNSS module, and external USB GNSS module. Specifically, **"internal GNSS" refers to the internal GNSS source integrated into the instrument at the factory; "EIO GNSS module" refers to the company's self-developed GNSS source that can be externally connected to the instrument; and "external USB GNSS module" refers to third-party GNSS modules that support serial communication.** Additionally, this section explains how to use the 1PPS trigger from the internal GNSS module and the 10 MHz reference clock from high-quality GNSS modules.

**Table 4 Description of GNSS parameters**

| No. | Parameter                   | Description                                                                                                                                                                                                                                                                 |
|-----|-----------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 1   | GNSS Source                 | Internal GNSS: Uses the internal GNSS module of the instrument.<br>External EIO GNSS module: Uses the manufacturer's dedicated external EIO GNSS expansion module.<br>External USB GNSS module: Uses a third-party GNSS module that supports standard serial communication. |
| 2   | Baud Rate                   | Serial port baud rate for the external GNSS module.<br>Required only when using an external GNSS module.                                                                                                                                                                    |
| 3   | Antenna                     | Required only when using the external EIO GNSS module.<br>External: Connect the external GNSS antenna to the MMCX (F) antenna connector on the EIO GNSS module.<br>On-board: Connect the external GNSS antenna to the IPEX (M) antenna connector on the EIO GNSS module.    |
| 4   | XPPS Out                    | On: Outputs the XPPS pulse signal<br>Off: Forces the GNSS module's XPPS output function to be disabled                                                                                                                                                                      |
| 5   | XPPS                        | Adjust the output pulse frequency of the GNSS module, in Hz.<br>Default value: 1Hz, which outputs a 1PPS signal. If set to 0.5Hz, a pulse is output every 2 seconds.                                                                                                        |
| 6   | Format                      | Provides two formats: Local Time and UTC Time.                                                                                                                                                                                                                              |
| 7   | SatNum                      | Number of satellites currently positioned.                                                                                                                                                                                                                                  |
| 8   | SNR(Max)                    | Maximum signal-to-noise ratio of positioned satellites.                                                                                                                                                                                                                     |
| 9   | SNR(Min)                    | Minimum signal-to-noise ratio of positioned satellites.                                                                                                                                                                                                                     |
| 10  | SNR(Avg)                    | Average signal-to-noise ratio of positioned satellites.                                                                                                                                                                                                                     |
| 11  | Reference Frequency Offset  | Displays the frequency offset between the internal GNSS clock and the device.                                                                                                                                                                                               |
| 12  | Reference Clock Calibration | Calibrate the internal reference clock frequency based on the measured reference clock frequency offset.                                                                                                                                                                    |

### 5.9.1 Using the internal GNSS Source

**PX, NX, and the new SAN series instruments feature a internal GNSS source by default.**

1. Connect the GNSS antenna to the GNSS antenna port of the device;
2. Click "System" -> "GNSS Info", and set "GNSS Source" to "Internal GNSS";
3. Wait 1 to 3 minutes for the GNSS to lock, you can judge whether the GNSS is locked or not according to the GNSS lock logo in the status bar information, after locking the GNSS lock logo is green, if it is grey, then it is not locked. see table 4 for the explanation of the parameters in the GNSS information pop-up window.



Figure 5 Use the internal GNSS source

### 5.9.2 Using the External EIO GNSS Module

**Both USB and Ethernet-based instruments support the external EIO GNSS module. Before starting the software, please ensure that the EIO GNSS module, the instrument, and the external GNSS antenna are properly connected; otherwise, the software will not be able to identify the GNSS module.**

1. Connect the EIO GNSS module to the AUXIO port of the instrument using a 14-pin ribbon cable, and connect the external GNSS antenna to the external antenna connector of the EIO GNSS module.
2. Start the software, set "GNSS Source" to "External EIO GNSS Module", and set "Antenna" to "External". Wait for 1-3 minutes. If the status in the bottom-left corner of the "GNSS Info" pop-up window changes from "Searching" to "Locked", the GNSS lock is successful.
3. When using a high-quality EIO GNSS module, set "DOCXO" to "Lock Mode" in the "GNSS Info" pop-up window. Wait for 5-10 minutes. If "DOCXO Locked" appears in the GNSS Info box, the DOCXO lock is successful.

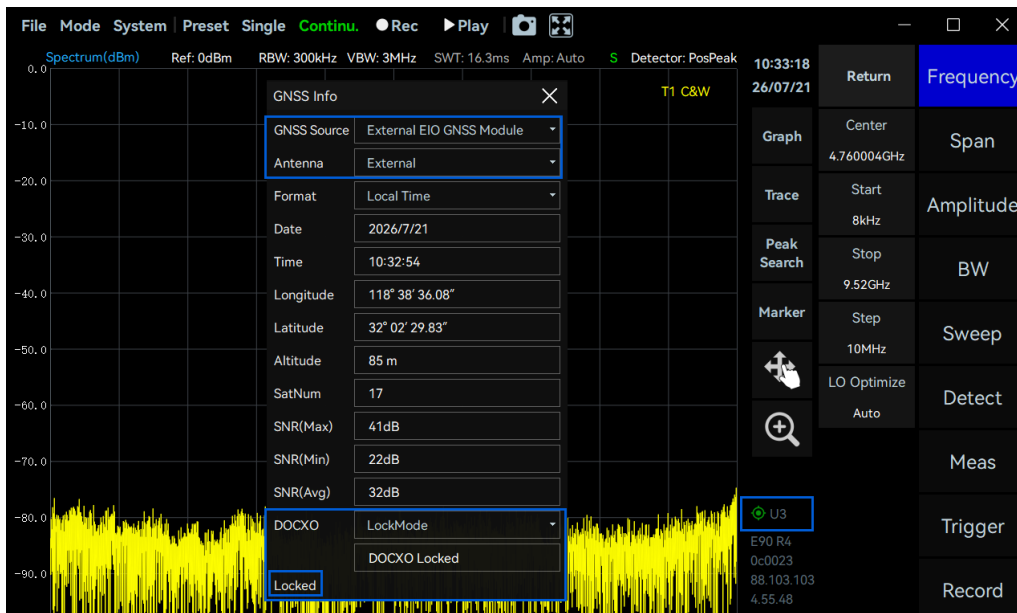


figure 6 Use the External EIO GNSS Module

### 5.9.3 Using the External USB GNSS Module

1. Connect the external GNSS module to the USB port of the PX series instrument or the host computer of the SA/NX series instrument using a USB-to-serial cable;
2. Click "System" -> "GNSS Info";
3. In the pop-up window, set "GNSS Source" to "External USB GNSS Module";
4. Click the "Refresh" button in the "COM Device" field, and select the newly identified "ttyACMX" or "COMX" device;
5. Set the "Baud Rate" to the actual output of the GNSS module (e.g., "9600"), and click the "Connect" button below;
6. The instrument will parse and display the received GNSS positioning information. For the parameter definitions in the GNSS Information pop-up window, please refer to [Table 4](#).



figure 7 Connect the external GNSS module

### 5.9.4 1PPS Trigger Using Default GNSS Source

The device supports 1PPS trigger signals provided by either the internal GNSS module or an external EIO GNSS module. The GNSS 1PPS trigger function is supported only in IQ Streaming Mode, Power Detection Mode, and Real-Time Spectrum Analysis Mode. This section uses the internal GNSS module as an example to describe in detail how to configure the 1PPS trigger function.

1. Refer to the [Using the internal GNSS Source](#) section on to ensure that the GNSS is locked;
2. Set "XPPS" to 1 Hz in the "GNSS Info";
3. Click "Mode" -> "IQStreaming" to switch to IQS mode;
4. Click "Next" -> "Trigger" in the main setup area, and set "TriggerSource" to "GNSS 1PPS" in the "Trigger" submenu to use the GNSS module 1PPS trigger.



Figure 8 Triggered using GNSS 1 PPS

### 5.9.5 Using the 10 MHz Reference Clock of the external EIO GNSS Module (Available Only on High-Quality GNSS Modules)

**Note:** Before launching the software, ensure that the EIO GNSS module, the instrument, and the external GNSS antenna are properly connected; otherwise, the software will not be able to identify the GNSS module.

1. Refer to the *Spectrum Analyzer Quick Start Guide* to properly connect the instrument, the EIO source, and the external GNSS antenna;
2. Refer to the section [Using the External EIO GNSS Module](#) to ensure that both GNSS and DOCXO are locked.
3. Set "RefCLKSource" to "Internal\_Premium" and "RefCLKFreq" to "10MHz" under the System submenu in the main settings area. At this time, the reference clock source is DOCXO.

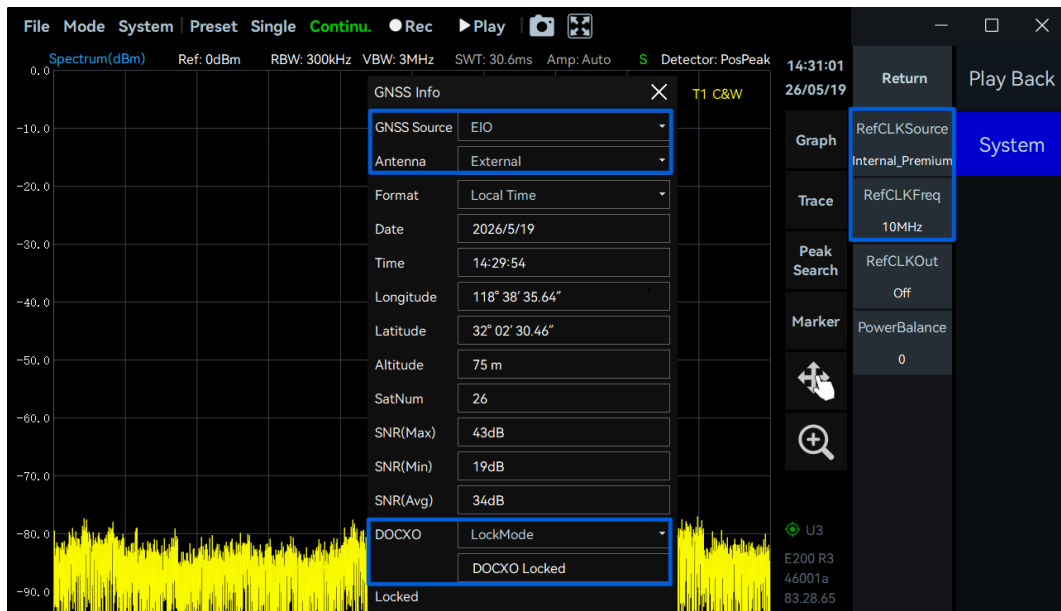


Figure 9 Using the 10 MHz reference clock of a high-quality GNSS module

### 5.9.6 Reference Clock Calibration

1. Refer to the [Using the internal GNSS source](#) section on to ensure that the GNSS is locked;
2. Click "Next" -> "System" in the main settings area to view the current reference clock frequency;
3. Click "Reference Clock Calibration" in the "GNSS Info" pop-up window. The instrument will complete a reference clock calibration based on the reference clock frequency offset measured by the GNSS.

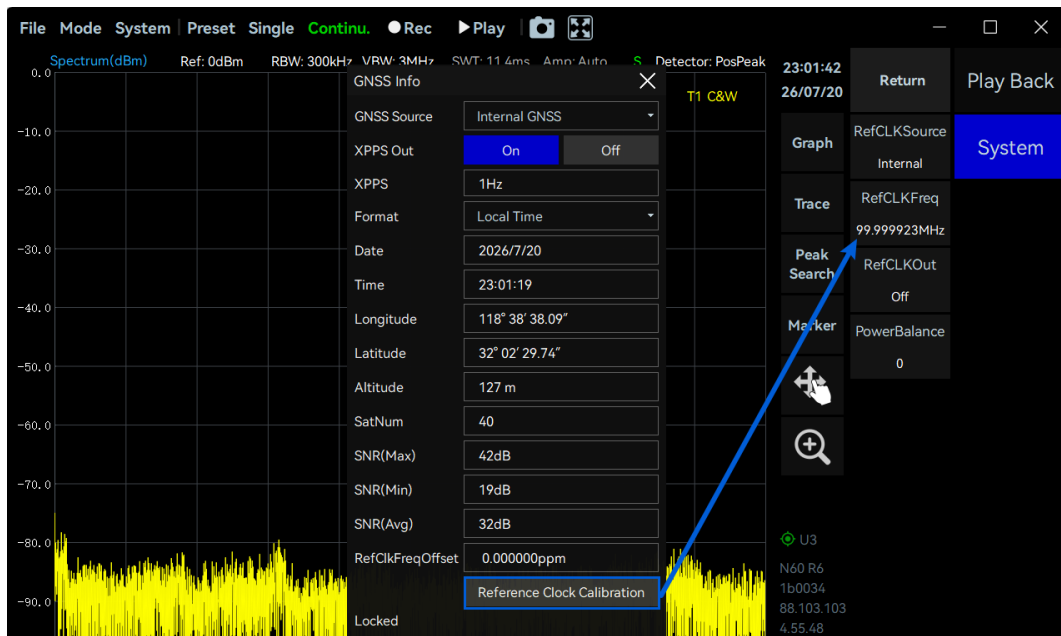


figure 10 Reference Clock Calibration

### 5.10 GPIO Output Level Control

After connecting the instrument to the corresponding EIO expansion board, click "System" -> "GPIO" in the menu bar to control the output levels of different GPIO interfaces. "On" indicates a high level, and "Off" indicates a low level. The interface definitions of the EIO expansion board are shown in the table below.

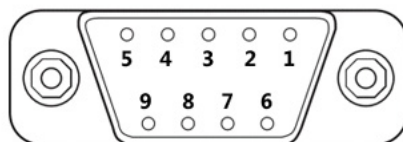


Figure 11 EIO Expansion Board Interface Diagram

**Table 5 EIO Expansion Board Interface Pin Description**

| Pin | Description |
|-----|-------------|
| 1   | GPIO0       |
| 2   | GPIO2       |
| 3   | GPIO4       |
| 4   | GPIO6       |
| 5   | GND         |
| 6   | GPIO1       |
| 7   | GPIO3       |
| 8   | GPIO5       |
| 9   | GPIO7       |

### 5.11 Viewing Instrument Information

Click "System" -> "About" in the menu bar, the UID number and firmware version of the current instrument will be displayed in the pop-up window.

### 5.12 Preset

Click the "Preset" button in the menu bar to restore the current software configuration to the default initial state of the instrument.

### 5.13 Single or Continuous Preview

Single preview: click "Single", Continuous preview: click "Continu.".

### 5.14 Quick Record and Playback

- **Recording:** Click "Rec" to start recording data, and click "Stop" to stop recording.
- **Playback:** Click "Play" in the menu bar to play back the last recorded data, and click "Pause" to pause the playback. Click the "Continu." button in the menu bar to resume normal data acquisition and display.

### 5.15 Hide Panel

Click the hide icon "☒" in the menu bar to hide the main settings menu and expand the display area. This function is only available in Tablet Mode.

### 5.16 Y-Axis Scale Zoom

Click "Graph" -> "Scale/Div" in the chart settings area to modify the dB value per division, thereby adjusting the vertical display range of the trace.

For PX series instruments, the Y-axis scale can also be adjusted in the following way:

Click the interactive mode button  in the chart setting area, then use touch gestures on the touchscreen:

- Spread two fingers vertically: Decrease the dB value per division;
- Pinch two fingers vertically: Increase the dB value per division.

### 5.17 Offset

The display offset of the trace can be adjusted in any of the following ways:

1. Click "Graph" -> "Offset" in the chart setting area, and enter the offset value in the offset setting interface, where a positive value indicates that the trace is offset downward and a negative value indicates that the trace is offset upward.
2. Click  in the chart settings panel to enable manual adjustment. Once enabled, press and drag the trace up or down to quickly adjust its display position.

You can later restore the default position via "Graph" -> "Reset Scale".

### 5.18 Switch X-Axis scale

Click the chart display area "Graph" -> "XScale" to display the X-axis of the spectrum either in "Lin" (Linear) or "Log" (Logarithmic) mode.

### 5.19 Display Line

Click "Graph" -> "Line" to enable a configurable visual reference line. Set the "LinePos" value to adjust its position on the y-axis.

### 5.20 Setting Chart Units

Click "Graph" -> "Units" to set the display units of the graph, including dBm, dBmV, dBmA, W, V, A, dBuV, dBuA and dBpW.

### 5.21 Spectrogram

Only the standard spectrum analysis, IQ streaming, and Real-Time spectrum analysis modes support the spectrogram display function. A description of each control in the spectrogram settings interface is provided in the table below:

**Table 6 Description of Spectrogram Controls**

| Graph Setting Area |                                                                                                |
|--------------------|------------------------------------------------------------------------------------------------|
| Scan Depth         | The time length cached on the y-axis of the spectrogram<br>Cache limit: 8000 lines of pixels   |
| Time Density       | The refresh rate of the spectrogram<br>When set to 100, scrolls 100 lines of pixels per second |
| Color              | Sets the color gradient for the spectrogram                                                    |

1. Click "Graph" -> "Spectrogram" to create a spectrogram corresponding to the spectrum;
2. Click the Spectrogram, switch to the corresponding chart setting area of the spectrogram, and then click "Graph" to enter the spectrogram setting interface;
3. "Export Image" can export the current spectrogram in PNG format to the ["/images"](#) folder, "DataExport" can export the current cached data not exceeding the scan depth to the ["/data"](#) folder in CSV format, and the exported data is sorted in reverse chronological order.

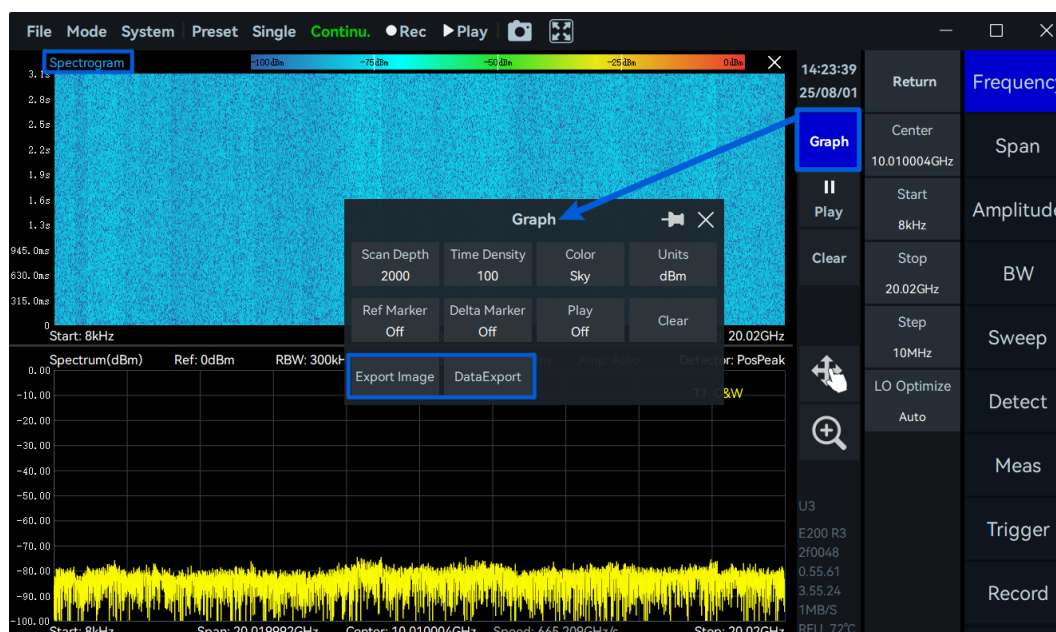


Figure 12 Enable Spectrogram

4. The Power range corresponding to the Spectrogram's Color Bar can be set by adjusting the "Offset" and "Scale/Div" parameters. The specific calculation rules are as follows:

- Color Bar Upper Limit = "Ref.Level" + "Offset"
- Color Bar Lower Limit = "Ref.Level" + "Offset" - 10 \* "Scale/Div"

## 5.22 Export Data

The PNG image or CSV data of the current chart can be exported in any of the following ways:  
Export as follows:

1. Click "Graph" -> "DataExport" in the setting area of the chart where the data is to be exported;
  2. Click the right mouse button in the chart display area, open the shortcut menu, select "DataExport".
- The "Image" option allows you to export the current chart as a PNG image file, which is saved to the ["/images"](#) folder by default;
  - The "Data" can export chart data to CSV file, default save to ["/reports"](#) folder.

## 5.23 Record and Playback

Please refer to table 6 for key parameters in record and playback function. The record file format description is provided in [Appendix 1](#) through [Appendix 5](#).

**Table 7 Record and playback parameter description**

| Record               |                                                                                                                                                                                                                                                                                                                                                                                     |
|----------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>RecordMode</b>    | FixedPoints: Allows presetting the number of recording points, recording duration, and file size limit. The actual recording duration cannot exceed the set "file size limit".<br>Adaptive: Requires manually controlling the recording duration of the file. (Note: In manual mode, the software will automatically stop recording if the file size exceeds the "file size limit") |
| <b>RecordTime</b>    | Set the recording duration, only effective when the record mode is "FixedPoints"                                                                                                                                                                                                                                                                                                    |
| <b>FileSizeLimit</b> | The storage size limit for a single recording file                                                                                                                                                                                                                                                                                                                                  |

|                     |                                       |
|---------------------|---------------------------------------|
| <b>Diskcapacity</b> | The remaining and total disk capacity |
| <b>Play Back</b>    |                                       |
| <b>Last frame</b>   | Rewind by one frame                   |
| <b>Next frame</b>   | Fast forward by one frame.            |
| <b>Back</b>         | Rewind by multiple frames.            |
| <b>Forward</b>      | Fast forward by multiple frames.      |

## 1. Data Recording

- 1). Click "Record"-> "RecordMode" in the main setting area and select the desired record mode;
- 2). Click "REC File Path" to set the storage location of the log files, the default path is ["/data"](#) folder, users can also customize the storage path;
- 3). In "Fixed" mode, click "Record" to automatically record data of a preset size. In "Manual" mode, you can manually control the recording duration by clicking "Record" and "Stop". Automatically stops recording when the file size exceeds the file size limit.

## 2. Data Playback

- 1). Click "Play Back" -> "Open File" in the main setting area, and select the record file to be played back in the pop-up window.
- 2). Click "Playback" to start playback, click "Pause" to stop playback, click "Stop" to exit the playback interface to resume data acquisition, and enable Turn on "Auto Loop" to loop back the record file.

### 5.24 Graph Zoom Function

The chart zoom function can be used to view detailed information in a local region of a spectrum or time-domain plot. The instrument provides two zoom methods: Zoom scaling and magnifier zoom, allowing users to flexibly choose according to their needs.

#### 5.24.1 Zoom Function

##### 1. Spectrum Zoom (Only in SWP mode)

- 1). Click "Graph" -> "Zoom";
- 2). Click to select "Spec zoom", click "Graph", set the frequency range to be zoomed in the pop-up submenu, or directly drag the zoom box and its edges in the spectrum graph to adjust the position and zoom area.



Figure 13 Spectrum zoom in SWP mode

## 2. Time Domain Zoom (Only in IQvT, PvT, and DET Modes)

### 1). IQvT and PvT

In IQS mode, click "IQvT" or "PvT" in the main setting area, select the corresponding channel, open "Analyze" and "Zoom". Open "Analyze" and "Zoom", adjust the zoom area by holding down the zoom area and sliding the zoom frame, or holding down the zoom border and dragging it left and right.

### 2). DET mode

a) Click on "Graph" and open "Zoom" in the pop-up submenu;

b) Slide the zoom frame by holding down the zoom area, drag the zoom border left and right, select the zoom graph "PvT Zoom", and click "Graph" to set the "TimeCenter" and "TimeRange". You can adjust the zoom area.

## 5.24.2 Magnifying Glass Function

1. Click on the magnifying glass button "🔍" to frame the area of interest;
2. A thumbnail view will be displayed in the upper right corner of the main interface, showing the complete trace and the position of the zoomed-in area in the global picture;
3. You can quickly switch the position of the zoomed-in area by dragging the red box in the thumbnail, or you can re-select a new area to zoom in;
4. Click the Zoom button again to exit the zoomed-in view and restore the original trace display.

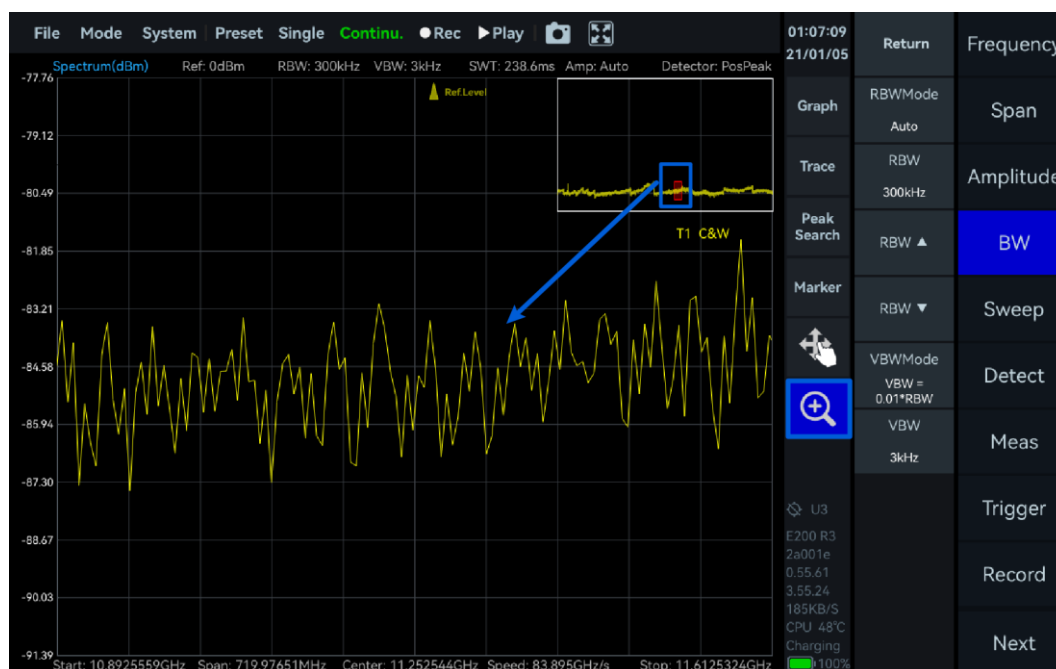


Figure 14 Magnifying Glass Zoom in SWP Working Mode

### 5.24.3 Interactive Zoom(PX series only)

Click the interactive mode button "👉" in the chart setting area, then use touch gestures on the touchscreen:

- Swipe left or right with one finger: Adjust the center frequency;
- Spread two fingers horizontally: Decrease the span;
- Pinch two fingers horizontally: Increase the span.

### 5.25 Trace settings

Click on "Trace" in the chart settings area and see the following table for a description of the parameters in the additional menu:

**Table 8 Trace Control Parameter Description**

| Trace                  |                                                                                                             |
|------------------------|-------------------------------------------------------------------------------------------------------------|
| <b>Enabled</b>         | On: Turn on the traces of the corresponding labels, the upper limit is 4.                                   |
| <b>Type</b>            | ClearWrite, MaxHold, MinHold and Average                                                                    |
| <b>Avg</b>             | Setting the average number of times the average type of trace is averaged                                   |
| <b>StateReset</b>      | Clears the current trace data and restarts the display according to the set trace type.                     |
| <b>Edit Lable</b>      | Modify trace name for user to edit and manage multiple traces.                                              |
| <b>Max/Avg/C&amp;W</b> | Simultaneously enable three traces for MaxHold, Average and ClearWrite                                      |
| <b>Max/Avg/Min</b>     | Simultaneously enable three traces for MaxHold, Average and MinHold                                         |
| <b>Reset</b>           | Resets the trace display method, clears all current trace data, and reverts to the default clear write type |

## 5.26 Maker Function

### 5.26.1 Create Markers

1. Create a Marker  
Double-click on the chart display area, or click on "PeakSearch" in the chart settings area to quickly bring up the reference marker.
2. Create multiple Markers  
Click the "Marker" submenu in the Chart Settings area, select the marker you want to create, and then click "Enable" to enable the selected marker.

### 5.26.2 Create Marker Pairs

Marker pairs can be created in any of the following ways (reference marker and difference marker as a group, current limit 5 groups):

1. In the "Marker" submenu, select the marker pairs you want to create (e.g., "M1R" and "M1D") and click on "Enable";
2. Right-click on the chart display area to open the shortcut menu and select "Create marker pair";
3. Click "Graph" -> "Marker Pair" in the Graph Settings area to quickly enable a pair of reference marker and difference marker, and click continuously to enable multiple pairs of markers.

### 5.26.3 Close Markers

1. Close a Single Marker  
In the "Marker" submenu, select the marker you want to disable and click "Enable" to disable the selected marker.
2. Close all Markers

All currently enabled markers can be cleared in one of the following ways.

- 1). Click "Graph" in the Chart Settings area and select "Clear All" in the pop-up window;
- 2). Click the right mouse button in the chart display area, open the shortcut menu, select "Clear all markers".

### 5.26.4 Change Markers Frequency

1. Manual Enter Frequency Value  
Click "Marker" submenu, select an enabled marker (e.g. M1R, M2R), click the "Freq:" area on the top of the pop-up window, and set the marker frequency value.
2. Drag Marker or Click to Jump
  - 1). Drag Marker: press and hold the marker and drag it to the desired position and then release it;
  - 2). Click to Jump: select the marker, then double-click on the target frequency point; the marker will automatically jump to that position.

### 5.26.5 Marker switching traces

Switching the marker trace can be achieved using either of the following methods:

1. Click "Marker" in the chart device area, select the target trace (e.g. switch from T1 to T2), the marker will automatically jump from T1 to the corresponding frequency position of T2;
2. Right-click on the graph display area to open the context menu and select "Marker trace" to

switch the target trace associated with the current marker.

### 5.26.6 Delta Marker

The delta marker must be used together with a reference marker to indicate the frequency difference, time difference, and amplitude difference relative to the reference marker.



Figure 15 Enable Delta Marker

### 5.26.7 Noise Density

After creating the marker, turn on "NoiseDensity" in the "Marker" section of the chart settings area to convert the original power values to power density per Hz.

### 5.26.8 Marker Peak Search

#### 1. Local peak search

Double-click on the chart near a local peak, or select the marker and click "Marker" -> "Local Peak".

#### 2. Global peak search

Click on "Peak Search" in the graph setting area to enable global peak search.

#### 3. Left and right peak search

##### 1). Enable Auto Parameter Setting

After enabling the cursor, click "Marker" -> "Left Peak" / "Right Peak" in the chart setting area. By default, "AutoParam" is enabled, and the software will calculate appropriate peak thresholds and peak offsets based on the noise floor and signal distribution of the current trace, so as to accurately identify valid local peaks.

##### 2). Set Custom Peak Threshold and Peak Offset

After the marker is enabled, click "Marker" -> "Advanced" in the chart setting area, set the "Threshold" and "Excursion" for left and right peak searching. After that, click "Left Peak" or "Right Peak", when a qualified signal is detected, the marker will automatically locate to the signal position.

- Peak Excursion: the minimum amplitude difference (dB) between the peak and the troughs on either side, used to determine if the peak is sufficiently prominent.

### 5.26.9 Marker to Center

The Marker to Centre function aligns the frequency of the current reference marker to the center of the chart, which can be achieved in any of the following ways:

1. After moving the reference marker to the target frequency point, click "Marker" -> "to Center" in the chart setting area;
2. After moving the reference marker to the target frequency point, click the right mouse button on the chart display area, open the shortcut menu and select "Marker to center".

### 5.26.10 Marker Switch to Mode

The Marker to Mode function quickly switches to other operating modes and sets the frequency at which the current reference marker is located as the center frequency of the new mode. This function can be realized in any of the following ways:

1. After moving the reference marker to the target frequency point, click "Marker" -> "Switch to" in the chart setting area, and select the target mode;
2. After moving the reference marker to the target frequency point, click the right mouse button in the chart display area, open the shortcut menu, select "Marker to Mode", and select the target mode.

### 5.26.11 Signal tracking

Signal tracking supported in standard spectrum analysis mode only.

1. Click "Marker" in the chart setting area, in the pop-up submenu, click "More", and then click "Advanced". Set the "Threshold" and "Shake Range" for the tracking signal (when the peak frequency jitters within this range, the frequency value will not be frequently aligned to the center position);



Figure 16 Set the Peak Threshold and Shake Range

- Click "Signal Track", the reference marker will search for peaks within the span at this time, and align the peak signal to the center frequency, when the frequency of the target signal drifts, the spectrometer will automatically adjust its own center frequency, so that the signal is always located in the center of the chart display area, which is convenient for the user to observe and analyze.



Figure 17 Frequency Tracking

Note: In general, this function only moves the frequency position and does not change the span. However, it is difficult to continue tracking signals with particularly large drift beyond the current span; for signals at the edge of the instrument's scanning range, because of frequency limitations, the span will be further reduced.

#### 5.26.12 Peak tracking

Click "Marker" -> "Peak Tracking" in the chart setting area. After enabling, the cursor will automatically locate and continuously track the maximum peak within the current sweep span. When the signal amplitude or frequency changes, the cursor position will update in real time, allowing the user to continuously observe variations in signal amplitude.

Note: The peak tracking function is only effective within the currently set sweep span. If the signal goes beyond this range, tracking will no longer continue.

#### 5.26.13 Peak table

The Peak Table function is only supported in Standard Spectrum Analysis Mode:

- Click "Marker" in the chart settings area. In the pop-up submenu, click "More", then "Advanced". Set the threshold for the Peak Table. For detailed setup instructions, see the [Signal Tracking](#) section;
- Click "Peak Table". The instrument will automatically detect and mark peak points that exceed the threshold within the current sweep span (up to 10 peaks). These peaks are listed in the Peak Table below the display area, showing the frequency and power of each peak in descending order of signal power, allowing users to quickly identify the main signals in the

spectrum.



Figure 18 Peak Table

5.27 Quick Parameter Setting

5.27.1 Parameter setting

Currently, quick settings are supported for the following commonly used parameters: Reference Level, RBW, VBW, Detector, Start frequency, Stop frequency, Span, Center frequency and other parameters. Users can tap the corresponding parameter on the screen and directly enter a value to modify it.

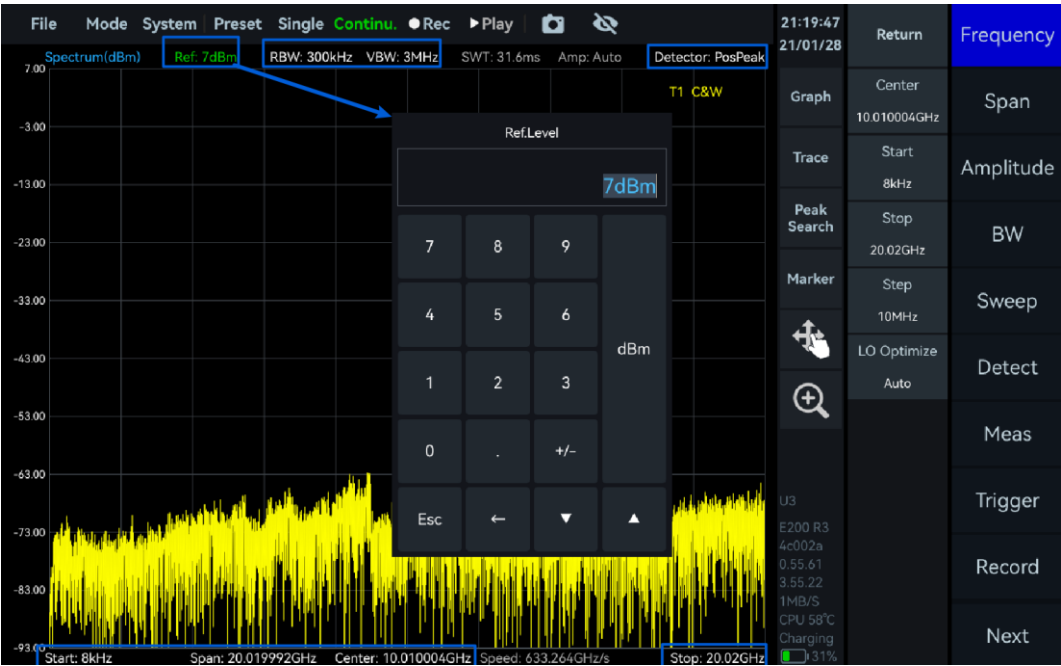


Figure 19 Setting Quick Parameters

In addition to entering values, the center frequency and span can also be quickly modified in the following ways:

- Center Frequency: Click the interactive mode button " " in the chart settings area, then press and drag the trace left or right.
- Span: Click the interactive mode button " " in the chart settings area, then scroll the mouse wheel. (Note: This quick method is supported in GUI version 3.55.28 and above.)

### 5.27.2 Parameter display

In addition to the quick parameterization, this area also supports the display of some of the key parameters during the measurement:

- SWT: Scan time for a single trace in the current configuration
- Amp: Preamplifier enabled status
- Spurious Suppression Label: Displays the spurious suppression mode in the current configuration (Note: Supported when GUI version is 3.55.26 and above)
  - "S" Indicates Standard Spurious Rejection
  - "E" Indicates Enhanced Spurious Suppression
  - Blank Indicates spurious suppression is not enabled
- Speed: the width of the spectrum swept per unit time in the current configuration (Hz/s)

### 5.28 Modifying the IQSampleRate

In IQ streaming mode, click "BW" in the main setup area and modify the value of "IQSampleRate" in the submenu to modify the sampling rate of the instrument.

To ensure the accuracy and repeatability of spectrum measurements, the instrument provides an amplitude correction function, which supports the user to compensate by manually inputting external gain/loss and importing the frequency response correction table. Currently, the amplitude correction function is only supported in spectrum analysis mode.

### 5.29 Amplitude Correction

To ensure the accuracy and repeatability of spectrum measurements, the instrument provides an amplitude correction function, which supports the user to compensate by manually inputting external gain/loss and importing the frequency response correction table. Currently, the amplitude correction function is only supported in spectrum analysis mode.

#### 5.29.1 Correction Rules

- Between the start frequency and the first compensation point in the current span, compensation is performed according to the offset value of the first frequency point;
- Between multiple compensation points, compensation is performed by linear interpolation based on the frequency data in the correction table;
- Between the last compensation point and the termination frequency, according to the offset value of the last frequency point.

#### 5.29.2 Amplitude Correction Example

Take the 1 GHz to 3 GHz band to compensate for -20 dB, the 3 GHz to 5 GHz band to perform -20 dB to +10 dB interpolation compensation, and the 5 GHz to 7 GHz band to compensate for 10 dB as an example, the operation steps are as follows:

1. Click "Frequency" and set "Start Frequency" to "1 GHz" and "Stop Frequency" to "7 GHz";

2. Click "System" -> "Amplitude Correction" in the menu bar;
3. Enable the amplitude correction function in the pop-up window, and then click "Add" to add one frequency correction item at a time;
4. Set Frequency 1 to "3 GHz" and Offset 1 to "-20 dB", click "Add" again and set Frequency 2 to "5 GHz" and Offset 2 to "10 dB";
5. Click "Apply" in the bottom right corner of the pop-up window to apply the amplitude correction function;



Figure 20 Amplitude correction application

6. Users can export the current correction configuration to an Excel table file via "Export" in the pop-up window, and the default export is to the ["/data"](#) folder;
7. The user can also customize the amplitude correction table according to the format of the exported configuration and import it using the "Import" button.

### 5.30 Antenna Attitude

In software with GUI version 4.55.44 and above, an antenna attitude function has been added. When an HDA-series handheld directional antenna that supports this function is connected, the software can display the antenna's azimuth, elevation, and polarization angle in real time to describe the spatial orientation and body attitude of the directional antenna during measurement.

#### 5.30.1 Interface Description

The interface is used to display the current attitude information of the HDA-series handheld directional antenna. It mainly consists of an attitude indicator area, an electronic compass area, and a numerical display area, as shown in the figure below:

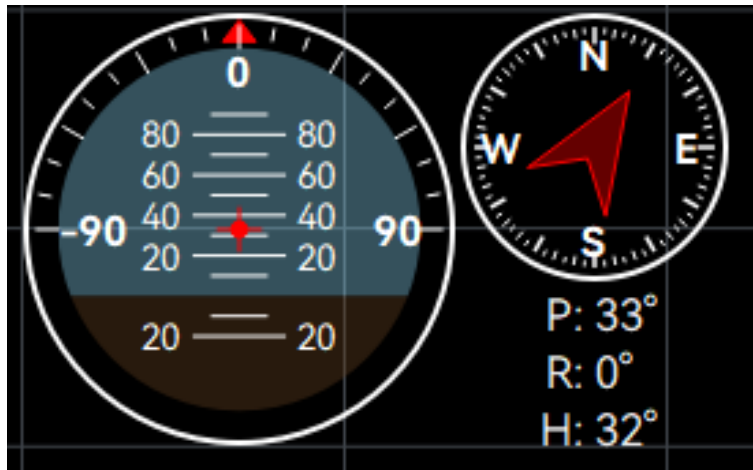


figure 21 Antenna attitude interface overview

On the left is the attitude indicator area, which displays the current elevation and polarization angle status of the antenna. The blue area represents the upward tilt direction, while the brown area represents the downward tilt direction. The angle scale line corresponding to the central red dot help indicate the current elevation angle. The red arrow on the periphery of the attitude indicator area is used to indicate the current polarization angle.

On the right is the electronic compass area, which displays the antenna's current azimuth. The red pointer indicates the horizontal orientation of the antenna's main receiving direction. The compass scale helps users determine the antenna's heading relative to the cardinal directions (North, East, South, and West).

At the bottom of the interface is the numerical display area, which shows the current values of elevation, polarization, and azimuth angle in real time.

### 5.30.2 Parameter Description

Table 9 Attitude Angle Parameter Description

| Attitude Angle      |                                                                                                                                                                                                                                                                                                                                                                                                                                   |
|---------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Elevation</b>    | The elevation angle is the upward or downward tilt of the antenna's main receiving direction relative to the horizontal plane. It describes the pointing state of the antenna in the vertical direction. The elevation angle changes when the antenna is tilted upward or pressed downward.<br>Display range: $-180^{\circ} \sim +180^{\circ}$                                                                                    |
| <b>Polarization</b> | The polarization angle is the attitude angle of the antenna after rotating around its main receiving direction axis. It describes the rotational state of the antenna's current receiving polarization direction. When the main receiving direction of the antenna remains unchanged, but the antenna body rotates around this axis, the polarization angle changes accordingly.<br>Display range: $-90^{\circ} \sim +90^{\circ}$ |
| <b>Avzimuth</b>     | The azimuth angle is the angle of the antenna's main receiving direction in the horizontal plane relative to the North direction. It describes the current horizontal pointing of the antenna. When the user rotates the antenna in the horizontal plane, the azimuth angle changes accordingly.<br>Display range: $0^{\circ} \sim 360^{\circ}$                                                                                   |

### 5.30.3 Steps for Using with HDA-series

1. Connect the communication interface of the HDA-series handheld directional antenna to the host computer using a USB Type-C to USB Type-A cable, and connect its RF output to the spectrum analyzer RF input.
2. Start the spectrum analyzer GUI software. Follow the pop-up "Antenna Direction Calibration" prompts to draw a figure-8 trajectory for calibration. Upon completion, the antenna attitude interface will automatically appear in the upper right corner of the measurement area (this interface can be freely dragged within the software).
3. Hold the HDA-series antenna normally, pointing the antenna's main receiving direction toward the area to be tested.
4. The antenna attitude interface will display the antenna's current elevation, polarization, and azimuth information in real time.
5. During the measurement, users can combine the spectrum amplitude or field strength variations with the current antenna attitude information to assist in determining the antenna's pointing state and the possible direction of the signal source.
6. To close the antenna attitude interface when it is not needed, select "System" -> "Antenna Attitude" from the menu bar. If you need to re-enable it later, you can restart it using the same menu path.

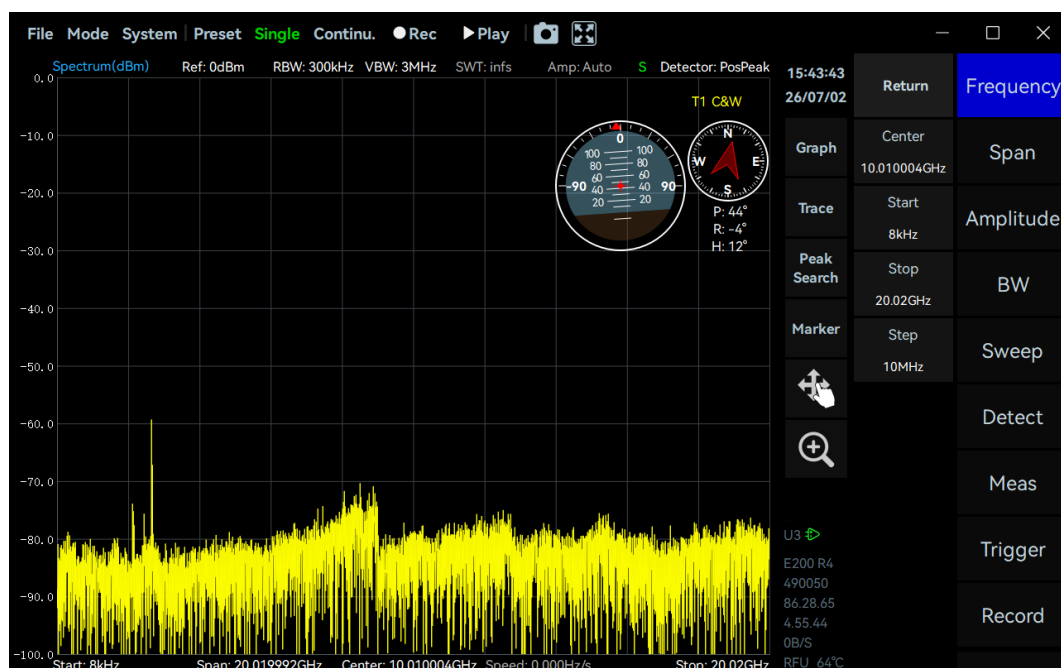


figure 22 Antenna attitude application

### 5.31 Display modes (only in SA/NX series)

The upper computer software of SA/NX supports three display modes: workstation single-column (default), workstation dual-column, and flat-panel mode; PX series instruments only support flat-panel mode. Users can choose the appropriate display mode according to their own needs.

**Table 10 Display Mode Lookup Table**

| Display Mode               | Description                                                                                                                           |
|----------------------------|---------------------------------------------------------------------------------------------------------------------------------------|
| <b>Workstation One Col</b> | Single-column parameter display, providing more spectrum display space for focused spectrum observation.                              |
| <b>Workstation Two Col</b> | Two-column parameter display, allowing more convenient parameter settings and simultaneous viewing/comparison of multiple parameters. |
| <b>Tablet</b>              | Suitable for tablets and other mobile devices, featuring a clean interface and easy touch operation.                                  |

### 5.32 SCPI Remote Control

**GUI version 4.55.52** and later support SCPI remote control.

Before using SCPI, launch SASTudio4 and enable the function by selecting "System" -> "SCPI".

SASTudio4 must remain running during remote control. For details on SCPI commands, refer to the *SCPI Application Guide*.



**Figure 23 Enabling the SCPI Function**

## 6. Using of the SWP mode

This section highlights some of the important parameters and test methods of the standard spectrum analysis model.

### 6.1 Introduction to the General Parameters of the SWP Mode

The important parameters of the SWP mode are described in Table below.

**Table 11 Description of SWP Mode Parameters**

|                         |                                                                                                                                                                                                                                                                                                                                                                                                                       |
|-------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Frequency</b>        |                                                                                                                                                                                                                                                                                                                                                                                                                       |
| <b>LO Optimize</b>      | Auto: default low spurious mode;<br>Speed: high sweep speed mode;<br>Spur: low spurious mode;<br>PhaseNoise: low phase noise.                                                                                                                                                                                                                                                                                         |
| <b>Amplitude</b>        |                                                                                                                                                                                                                                                                                                                                                                                                                       |
| <b>PreAmplifier</b>     | Set the operation of the preamplifier:<br>Auto On: The preamplifier turns on automatically when the reference level is below approximately -30 dBm.<br>Forced Off: The preamplifier remains off regardless of the reference level.<br>Low Gain: The preamplifier operates in low gain mode.<br>Medium Gain: The preamplifier operates in medium gain mode.<br>High Gain: The preamplifier operates in high gain mode. |
| <b>GainStrategy</b>     | LowNoise: Focuses on low noise while keeping the noise floor flat.<br>HighLinearity: Focuses on high linearity while keeping the noise floor flat.                                                                                                                                                                                                                                                                    |
| <b>IFGainGrade</b>      | 0 to X steps, 3 dB gain difference per step<br>Increasing IF Gain Step: Reduces RF gain, raises noise floor, improves linearity, and reduces spurs.<br>Decreasing IF Gain Step: Increases RF gain, lowers noise floor, reduces linearity, and increases spurs.                                                                                                                                                        |
| <b>Atten</b>            | Step size 3 dB<br>Atten = -1 dB (default): No attenuation.<br>Atten ≥ 0 dB: Attenuation is enabled.                                                                                                                                                                                                                                                                                                                   |
| <b>Amplitude Offset</b> | Adjusts the amplitude range of the signal displayed on the spectrum analyzer without changing the actual signal value. By setting an offset, the displayed result on the device is modified.                                                                                                                                                                                                                          |
| <b>Auto Reference</b>   | Available only in standard spectrum analysis mode.<br>When enabled, the instrument automatically adjusts the reference level to ensure the signal trace is displayed within an appropriate range, preventing overload or an excessively low display.                                                                                                                                                                  |
| <b>IFAGC</b>            | IF AGC Control<br>On: Reduces IF gain when saturation occurs to prevent overload.<br>Off: Disables automatic gain control.                                                                                                                                                                                                                                                                                            |
| <b>AGC Target</b>       | When IF gain control is enabled, set the target power for IF AGC: range is 0 to -30 dBFS; the Target represents the dBFS level relative to ADC saturation.                                                                                                                                                                                                                                                            |

|                       |                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
|-----------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>AGC Period</b>     | <p>Set the AGC Execution Period. Value range: -1 s to +2147483 s.</p> <p>When the Period is set to a value less than 0, AGC will execute once before sampling, and will not execute during sampling.</p> <p>When the Period is set to 0, Dynamic AGC is enabled.</p> <p>When the Period is set to a value greater than 0, AGC will execute periodically according to the set period.</p>                                                                             |
| <b>IF Out</b>         | <p>IF Output Control:</p> <p>On: Enables IF output.</p> <p>Off: Disables IF output.</p>                                                                                                                                                                                                                                                                                                                                                                              |
| <b>Antenna Factor</b> | Used to compensate for the antenna's gain or attenuation, in order to convert the signal received by the antenna into the actual electric field strength.                                                                                                                                                                                                                                                                                                            |
| <b>Sweep</b>          |                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
| <b>SWTMode</b>        | <p>min SWT: minimum sweep time;</p> <p>min SWTx2: approximately 2 times of min SWT;</p> <p>min SWTx4: approximately 4 times of min SWT;</p> <p>min SWTx10: approximately 10 times of min SWT;</p> <p>min SWTx20: approximately 20 times of min SWT;</p> <p>min SWTx50: approximately 50 times of min SWT;</p> <p>min SWTxN: approximately N times of min SWT,</p> <p>N = SweepTimeMultiple;</p> <p>Manual: approximately equal to the target SweepTime.</p>          |
| <b>PointsStrategy</b> | <p>SweepSpeed: priority is given to the fastest sweep speed;</p> <p>PointsAccuracy: priority is given to ensuring that the number of trace points is close to the target.</p>                                                                                                                                                                                                                                                                                        |
| <b>SpurRejection</b>  | Bypass, Standard and Enhanced.                                                                                                                                                                                                                                                                                                                                                                                                                                       |
| <b>FFTExecution</b>   | Auto: automatically selects the CPU or FPGA for FFT calculation based on the settings (using CPU for RBW below 30 kHz and FPGA for RBW above 30 kHz), CPU preferred, FPGA preferred, CPU Low Occ, CPU Mid Occ, CPU High Occ, FPGA only.                                                                                                                                                                                                                              |
| <b>Window</b>         | <p>FlatTop Window: higher amplitude accuracy.</p> <p>B-Nuttal Window: greater frequency selectivity.</p> <p>LowSideLobe Window: higher accuracy in measuring low-frequency signals.</p> <p>Rectangular Window: highest frequency resolution.</p> <p>Kaiser Window: <math>\beta = 7.6</math>.</p>                                                                                                                                                                     |
| <b>System</b>         |                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
| <b>RefCLKSource</b>   | <p>When using an external reference clock source, set the reference clock frequency to 10MHz.</p> <p>Internal: Use the internal reference clock.</p> <p>External: Use the external reference clock; if unavailable, automatically switches to the internal clock.</p> <p>External_Forced: An external reference clock must be connected. If not, the system will not switch to the internal clock, and an unlocked clock may result in unstable received signals</p> |
| <b>RefCLKOut</b>      | <p>All-New PXN and SAN series: When enabled, outputs a 100 MHz reference clock.</p> <p>Others: When enabled, outputs a 10 MHz reference clock.</p>                                                                                                                                                                                                                                                                                                                   |

## 6.2 Channel Power

As an example, a BPSK signal with a carrier frequency of 1 GHz, a power of -20 dBm and a symbol rate of 1 MHz is tested.

### 6.2.1 Parameters description

Only some of the important parameters are described here: the important parameters in the channel power measurement section are shown in Table below.

**Table 12 Description of Channel Power Measurement Parameters**

| Channel Power    |                                                                                                           |
|------------------|-----------------------------------------------------------------------------------------------------------|
| <b>Meas BW</b>   | The bandwidth of the channel to be measured; channel power is the integrated power within this bandwidth. |
| <b>SpanPower</b> | The measurement bandwidth to the current span and calculates the channel power within this range.         |

### 6.2.2 Procedure

1. Set "Center" to 1 GHz and "Ref.Level" to 0 dBm, click "Meas" menu and select "ChannelPower";
2. The software will automatically configure the default parameters, and the test results are shown below. The upper left corner of the measurement box shows the channel power value. In the lower "ChannelPower" column, you can also view the Meas BW, ChannelPower and Power Density values;
3. You can adjust the channel center frequency (press and hold the measurement area and slide to select), measurement bandwidth (press and hold the measurement border and drag left and right or adjust the Meas BW setting), and also modify the parameters such as "Center", "Span", "Ref.Level" and "RBW" in the main setting area to suit different signals.



Figure 24 Measurement of ChannelPower

6.3 Occupied Bandwidth

As an example, a BPSK signal with a carrier frequency of 1 GHz, a power of -20 dBm and a symbol rate of 1 MHz is tested.

6.3.1 Parameters description

Only some of the important parameters are described here: some of the important parameters of the occupied bandwidth measurement are shown in Table below.

Table 13 Description of OBW Parameters

| OBW    |                                     |
|--------|-------------------------------------|
| Method | XdB, Percentage                     |
| XdB/%  | Set specific XdB values/percentages |

6.3.2 Procedure

- 1. Set "Center " to 1 GHz and "Ref.Level" to 0 dBm, click "Meas" menu and select "OBW" in the submenu;
- 2. Click on "BW" and set "RBW" to 50 kHz;
- 3. The software will automatically configure the measurement parameters, and the measurement results are shown in the figure. You can see the occupied bandwidth value in the lower "OBW" column;
- 4. You can also modify the parameters such as "Center ", "Span", "Ref.Level" and "RBW", etc. in the main setup area to suit the measurement of different signals.

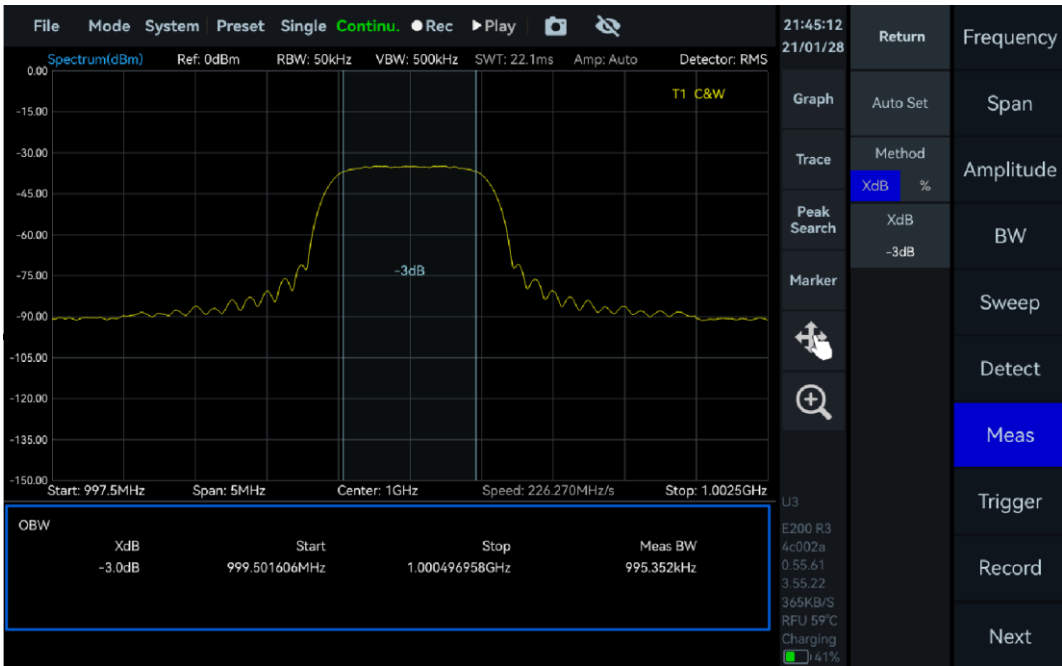


Figure 25 Measurement of OBW

6.4 Adjacent Channel Power Ratio (ACPR)

As an example, a BPSK signal with a carrier frequency of 1 GHz, a power of -20 dBm and a symbol rate of 1 MHz is tested.

6.4.1 Parameters description

Only some of the important parameters are described here: some of the important parameters of the adjacent channel power ratio measurement are shown in Table below.

Table 14 Description of ACPR Measurement Parameters

| ACPR  |                                                                                   |
|-------|-----------------------------------------------------------------------------------|
| Space | Setting the frequency interval between the main channel and the adjacent channel. |
| Count | Set the number of adjacent pairs, upper limit 2 pairs.                            |

6.4.2 Procedure

1. Set "Center" to 1 GHz and "Ref.Level" to 0 dBm, click "Meas" menu and select "ACPR" in the submenu;
2. The software will automatically configure the default parameters and the test results are shown below. The top green channel bandwidth is the power value of each channel. You can also check the Adj Center, Adj Power and Adj Ratio in the "ACPR" column at the bottom;
3. You can set the center frequency of the main channel, the bandwidth of each channel, the adjacent channel spacing and the number of adjacent channel pairs, and you can also modify the parameters such as "Center", "Span", "Ref.Level" and "RBW", etc. in the main setting area to suit the measurement of different signals.



Figure 26 Measurement of ACPR

## 6.5 IP3/IM3

Example of testing IP3/IM3 at the 1 GHz frequency point.

### 6.5.1 Parameters description

Only some of the important parameters are described here: Some of the important parameters for IP3/IM3 measurements are shown in Table below.

**Table 15 Description of IP3/IM3 Measurement Parameters**

| IP3/IM3                     |                                                                    |
|-----------------------------|--------------------------------------------------------------------|
| LowTone<br>Frequency/Power  | Frequency/Power of the input low-frequency signal.                 |
| HighTone<br>Frequency/Power | Frequency/Power of the input high-frequency signal.                |
| LowIM3P<br>Frequency/Power  | Frequency/Power of the intermodulation-generated low-side signal.  |
| HighIM3P<br>Frequency/Power | Frequency/Power of the intermodulation-generated high-side signal. |
| TonePowerDiff               | High and low frequency power difference of the input signal.       |

### 6.5.2 Procedure

1. Combine the signals with a center frequency of 999 MHz and an amplitude of 0 dBm and a center frequency of 1.001 GHz and an amplitude of 0 dBm into a single signal by means of two signal sources and combiners, and input them into the instrument;
2. Set the "Center" of the instrument to 1 GHz and the "Ref.Level" to 0 dBm, click the "Meas" menu and select "IM3";
3. Adjust the signal power so that the third-order intermodulation interference signal appears approximately 6 dB below the reference level in the spectrum;
4. The software will automatically configure the default parameters and the test results are shown below. The IP3 test results can be viewed in the "IM3" column below.

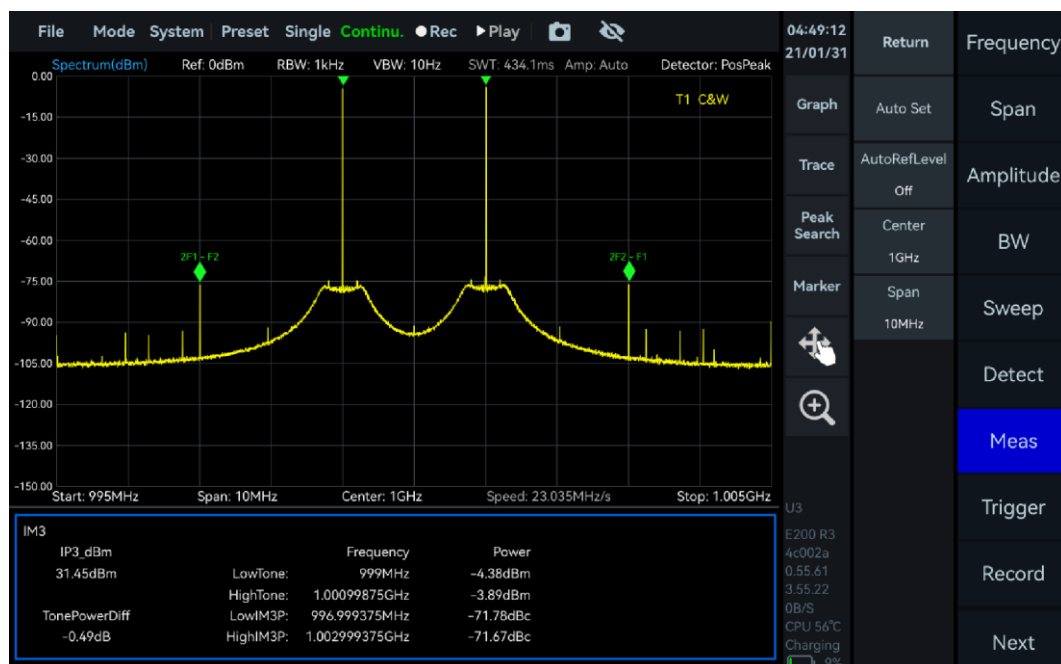


Figure 27 Measurement of IP3/IM3

## 6.6 SEM

The Spectrum Emission Mask (SEM) is a measurement function used to evaluate whether a wireless signal has excessive emissions or spurious signals outside its operating frequency band.

As an example, this function can be used to assess whether an IEEE 802.11ac signal with a frequency of 1 GHz and a power level of -20 dBm complies with the standard.

### 6.6.1 Parameters description

Only some of the important parameters are described here: some of the important parameters for SEM measurements are shown in Table below.

**Table 16 Description of SEM Measurement Parameters**

| SEM                  |                                                                                                                                                                                                                                              |                                                                                                                                                                                                                                                                                  |
|----------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Auto Set</b>      | Linkage with peak reference type, automatically using the signal peak as the current relative reference when enabled.                                                                                                                        |                                                                                                                                                                                                                                                                                  |
| <b>Ref Set Type</b>  | Manual: When enabled, user-defined relative reference level.<br>Peak: When enabled, the peak of the current signal is used as the relative reference level.                                                                                  |                                                                                                                                                                                                                                                                                  |
| <b>Manual Ref</b>    | Sets the relative reference level value. This function only works when "Manual" is selected as the reference type The set manual reference value will be used as the reference for calculating the start/stop threshold in the offset table. |                                                                                                                                                                                                                                                                                  |
| <b>Offset Table</b>  | StarFreq/StopFreq                                                                                                                                                                                                                            | Set the upper offset band to indicate the offset distance relative to the center frequency. The system automatically generates upper and lower offset bands symmetrical to the center frequency, and up to 16 offset bands can be configured.                                    |
|                      | LimitStart/LimitStop                                                                                                                                                                                                                         | Setting the power limit of the signal in the corresponding upper and lower offset bands                                                                                                                                                                                          |
|                      | Mode                                                                                                                                                                                                                                         | Absolute: Measurement in absolute amplitude, based on the actual power value, independent of the reference value.<br>Relative: Measurement relative to a set "Manual" value, based on the reference value to calculate the power limit in the offset band.                       |
|                      | Priority                                                                                                                                                                                                                                     | Required: must meet the requirements of the template, if not, it will be regarded as a failure.<br>Suggested: recommended to meet the requirements of the template, if not, then prompt a warning.                                                                               |
|                      | Save Table                                                                                                                                                                                                                                   | Save the current measurement template<br>Default path: <a href="#">"/data"</a> .                                                                                                                                                                                                 |
|                      | Load Table                                                                                                                                                                                                                                   | Load user pre-stored measurement templates                                                                                                                                                                                                                                       |
|                      | Load Preset                                                                                                                                                                                                                                  | Select the appropriate template from the predefined templates provided with the device Template type: 802.11a/g, 802.11b, 802.11n (20MHz, 40MHz), 802.11ac (20MHz, 40MHz, 80MHz, 160MHz) AM NRSC, FM FCC 73.317, FM NRSC Hybrid, AM NRSC 5K Hybrid, AM NRSC 8K Hybrid, Bluetooth |
| <b>Export Result</b> | Export the measurement table below the trace as a table<br>Default path: <a href="#">"/reports"</a> .                                                                                                                                        |                                                                                                                                                                                                                                                                                  |

## 6.6.2 Procedure

1. Set the "Center" to 1 GHz and the "Ref.Level" to -20 dBm;
2. Click "Meas" and select "SEM" in the additional menu;
3. Click "Offset Table", select the "Load Preset" button in the pop-up window, and select the "802.11ac (20MHz)" template in the template list;
4. Click "BW", adjust "RBW" to "5 kHz" and "VBW Mode" to "VBW = 0.01 RBW";
5. Click "Sweep", set "SWTMode" in the additional menu to "minSWT×20", and set "Detector" to "Average";
6. The measurement results are shown in the figure below, the spectrum map will show whether this spectrum meets the requirements of the template, and the maximum margin on each offset band is shown in the table below the measurement results.



Figure 28 Measurement of SEM

## 6.7 Auto Reference Level

The Auto Reference Level function is used to automatically adjust the reference level of the instrument to ensure that the signal trace is within the appropriate display range to avoid the signal being out of range or displayed too low.

The following is an example of adjusting the power adjustment of a 1 GHz single tone signal:

1. Input a signal with a frequency of 1 GHz and a power of -35 dBm into the instrument;
2. Set the "Start Frequency" to 90 MHz and the "Stop Frequency" to 3 GHz;
3. Click "Amplitude" in the menu bar to enable the function of "Auto Reference Level";
4. The system will automatically adjust the reference level from 0 dBm to -30 dBm;
5. Modify the input signal power to 5 dBm, the reference level will be adjusted from -30 dBm to +10 dBm.

Note: The lower limit of the automatic reference level threshold is -70 dBm, the adjustment step is 10 dB/grade, the input signal should not exceed the corresponding loss power of each frequency band.

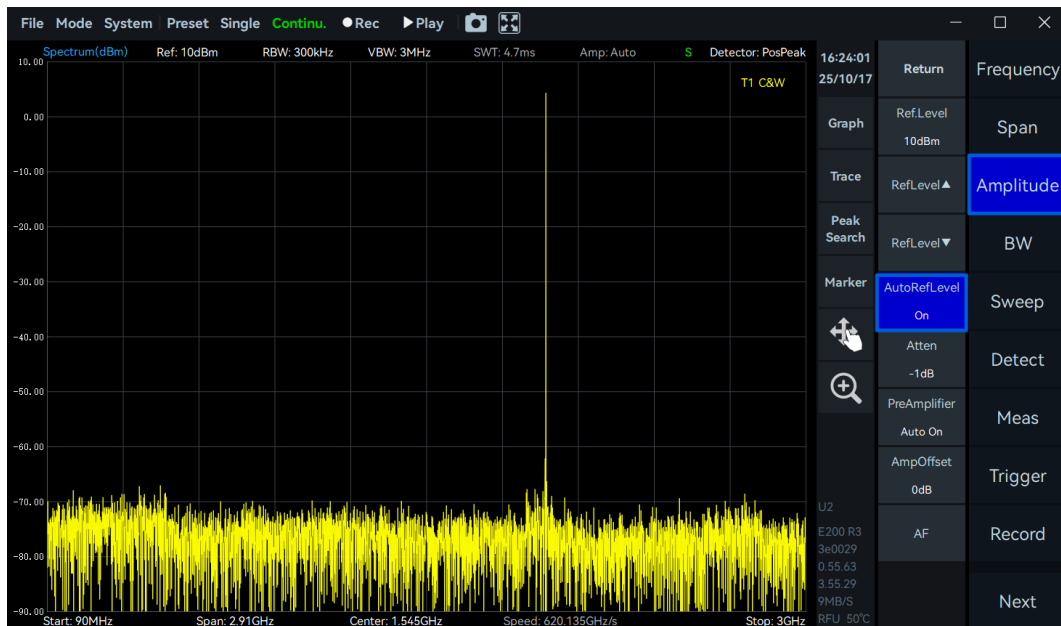


Figure 29 Enable Automatic Reference Level

## 6.8 Antenna Factor

In software versions 3.55.28 and above of the GUI, the Antenna Factor function has been added. It is used to compensate for the antenna's gain or attenuation and to convert the signal received by the antenna into the actual electric field strength.

### 6.8.1 Parameters description

Only some key parameters are explained here: the main parameters of the antenna factor are shown in Table below.

**Table 17 Description of Antenna factor Parameter**

| Antenna Factor |                                                                                                                                    |
|----------------|------------------------------------------------------------------------------------------------------------------------------------|
| Enable         | On: Activates the Antenna factor function.                                                                                         |
| Import         | Allows users to customize the Antenna Factor configuration according to the exported file format and import it into the system.    |
| Export         | Exports the current Antenna Factor configuration as an Excel file, with the default export path set to the "/data" folder          |
| Apply          | After setting or updating the Antenna Factor configuration, click the Apply button to make the configuration take effect           |
| Load           | When paired with the HDA-100 active directional antenna, no configuration is required and the antenna factor is loaded at a button |

### 6.8.2 Compensation Rules

- From the start frequency to the first compensation point within the current sweep span, compensation is applied using the factor of the first compensation point;
- Between multiple compensation points, compensation of the antenna factor is performed using linear interpolation based on the frequency point data in the correction table;
- From the last compensation point to the stop frequency, compensation is applied using the factor of the last compensation point.

### 6.8.3 Antenna Factor Configuration Example

For example, to configure compensation as follows: 17.5 dB for the 30 MHz to 50 MHz band, linear interpolation from 17.5 dB to 27.3 dB for the 50 MHz to 1 GHz band, and 27.3 dB for the 1 GHz to 2 GHz band, proceed with the following steps:

1. Click "Frequency", set "Start" to 30 MHz and "Stop" to 2 GHz;
2. Click "Amplitude" -> "Antenna Factor" in the menu bar;
3. In the pop-up window, enable "Enable", then click "Add". Each click allows you to add one frequency correction entry;
4. Set "Frequency 1" to "50 MHz" and "Factor 1" to "17.5 dB". Click "Add" again, then set "Frequency 2" to "1 GHz" and "Factor 2" to "27.3 dB";
5. Click "Apply" in the bottom-right corner of the pop-up window to apply the antenna factor compensation;
6. Users can also click "Export" to export the current configuration as an Excel file, which is saved by default in the `"/data"` folder;
7. If using antenna factor data provided by the manufacturer, you need to generate a correction table in the same format as the exported file so it can be recognized by the software, and then import it using the "Import" button.



Figure 30 Antenna Factor Configuration Example

### 6.8.4 Auto Load Antenna Factor

When paired with HDA-100 active directional antenna, there is no need to manually configure it, the system can automatically load the antenna factor, thus enhancing work efficiency. The specific steps are shown below:

1. Correctly connect the instrument and HDA-100 active directional antenna, and start the software;
2. Set the "Start Frequency" to 500 MHz and the "End Frequency" to 10 GHz;
3. Click "Amplitude" -> "Antenna Factor" in the menu bar;
4. Enable "Enable" in the pop-up window, and then click "Load", the system will load the antenna factor automatically.



Figure 31 With HDA-100: automatic loading of antenna factors

## 7. Using of the IQS mode

This chapter describes in detail some of the important parameters of the IQ streaming mode, and focuses on describing how to carry out further analyses of the time-domain IQ data acquired by the system, such as spectral analysis, time-domain analysis, power-time analysis, digital down-conversion, demodulation, etc.

### 7.1 Introduction to the General Parameters of The IQS mode

**Table 18 Description of IQS Mode Parameters**

| Frequency       |                                                                                                                                                       |
|-----------------|-------------------------------------------------------------------------------------------------------------------------------------------------------|
| LO Optimize     | Please refer to the parameter with the same name in the <a href="#">Introduction to the General Parameters of SWP Mode</a> .                          |
| BW              |                                                                                                                                                       |
| IQSampleRate    | ADC sampling rate, 110 MSPS to 130 MSPS can be set.                                                                                                   |
| AnalysisBw      | Display the equivalent sampling rate after extraction: Span * 0.8.                                                                                    |
| Span▲/▼         | Support increasing or decreasing the analysis bandwidth in powers of two.                                                                             |
| DataFormat      | 8-bit: Lower precision. When there is no signal, many zeros are likely to be captured.<br>16-bit: Default configuration.<br>32-bit: Higher precision. |
| Amplitude       |                                                                                                                                                       |
| PreAmplifier    | Please refer to the parameter with the same name in the <a href="#">Introduction to the General Parameters of SWP Mode</a> .                          |
| GainStrategy    |                                                                                                                                                       |
| IFGainGrade     |                                                                                                                                                       |
| Atten           |                                                                                                                                                       |
| AmpOffset       |                                                                                                                                                       |
| IFAGC           |                                                                                                                                                       |
| IFAGCTarget     |                                                                                                                                                       |
| IFOut           |                                                                                                                                                       |
| Current IF Gain | Unit: dB. Returns the current IF AGC gain, where positive values indicate amplification and negative values indicate attenuation.                     |
| Record          |                                                                                                                                                       |
| RecordMode      | Please refer to the parameter with the same name in the <a href="#">Recording and Playback</a> .                                                      |
| RecordTime      |                                                                                                                                                       |
| FileSizeLimit   |                                                                                                                                                       |
| Diskcapacotu    |                                                                                                                                                       |

## Playback

|                   |                                                                                                  |
|-------------------|--------------------------------------------------------------------------------------------------|
| <b>Last frame</b> | Please refer to the parameter with the same name in the <a href="#">Recording and Playback</a> . |
|-------------------|--------------------------------------------------------------------------------------------------|

|                   |
|-------------------|
| <b>Next frame</b> |
|-------------------|

|             |
|-------------|
| <b>Back</b> |
|-------------|

|                |
|----------------|
| <b>Forward</b> |
|----------------|

|               |
|---------------|
| <b>System</b> |
|---------------|

|                     |                                                                                                                              |
|---------------------|------------------------------------------------------------------------------------------------------------------------------|
| <b>RefCLKSource</b> | Please refer to the parameter with the same name in the <a href="#">Introduction to the General Parameters of SWP Mode</a> . |
| <b>RefCLKOut</b>    |                                                                                                                              |

## 7.2 IQ Streaming Working Mode Overview

The initial interface of the IQ Stream Mode consists of a Max Power vs. Time thumbnail, a spectrum plot, and a time-domain plot. Click "Next" in the main settings area, then click "Trigger". In the submenu, modify the "Preview Time" parameter to adjust the preview time range of the IQ stream in the Max Power vs. Time thumbnail.

The display ranges of the spectrum plot and the IQ time-domain plot are determined by the red selection boxes, "Spectrum-P" and "IQvT-P", in the Max Power vs. Time thumbnail. By adjusting the position and range of these selection boxes, you can observe IQ time-domain signals from different time segments, or perform spectrum analysis on IQ time-domain signals captured over different time periods.

## 7.3 Spectrum Analysis

### 7.3.1 Parameters description

Only some of the important parameters are described here: the important parameters in the spectrum analysis section are shown in Table 18.

**Table 19 Description of Spectrum Analysis Parameters**

#### Spectrum analysis

|               |                                                                                                                              |
|---------------|------------------------------------------------------------------------------------------------------------------------------|
| <b>Window</b> | Please refer to the parameter with the same name in the <a href="#">Introduction to the General Parameters of SWP Mode</a> . |
|---------------|------------------------------------------------------------------------------------------------------------------------------|

|                  |                                                                                                                                                              |
|------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Intercept</b> | Spectrum interception: e.g. Intercept = 0.8, displays 80% of the FFT spectrum analysis results in order to intercept the transition band spectral components |
|------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------|

### 7.3.2 Procedure

1. Click "FFT" in the main settings area and enable "Analyze". Drag the red selection box "Spectrum-P" in the Max Power vs. Time thumbnail, or adjust the values of "TimeStart" and "TimeLength" to perform spectrum analysis on IQ signals collected over different time segments. Adjust the values of "Center" in the "Frequency" submenu and "Span" in the "BW" submenu to change the center frequency and analysis bandwidth of the spectrum;
2. Use "FFTsize" to set the number of points for spectrum analysis, "Window" to select different window functions, "TraceDetector" to set different trace detectors, and "Intercept" to crop the displayed spectrum. When Intercept = 0.8, the transition band can be cropped.

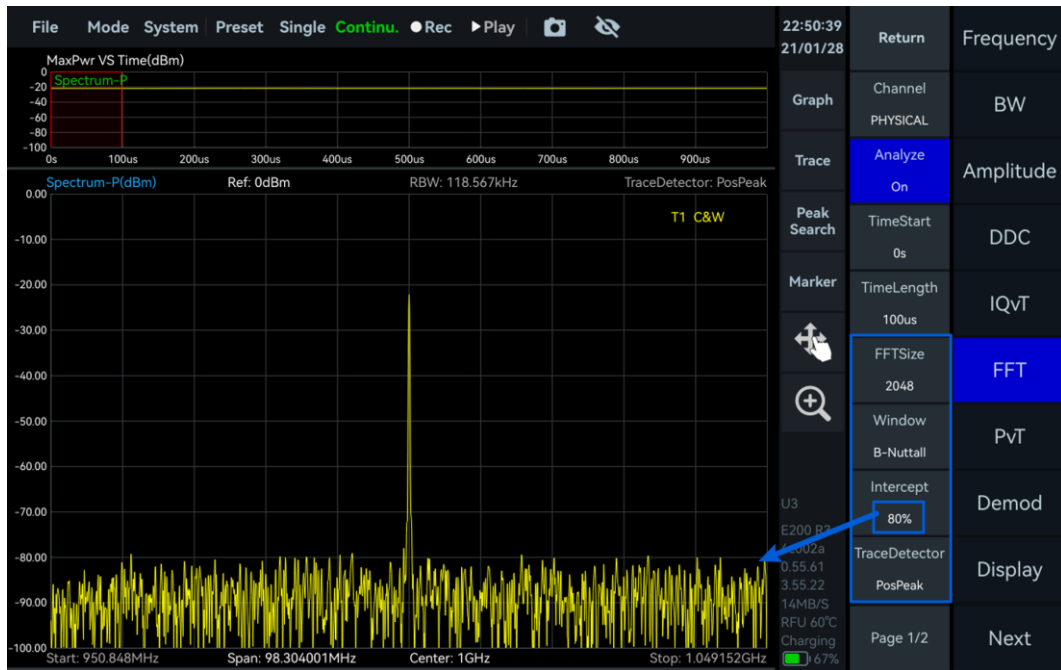


Figure 32 Spectrum analysis of IQ data

## 7.4 IQvT

### 7.4.1 Procedure

Click "IQvT" in the main settings area and enable "Analyze". Drag the red selection box "IQvT-P" in the Max Power vs. Time thumbnail, or adjust the values of "TimeStart" and "TimeLength". Then click "Auto Range" under "Graph" to perform time-domain analysis on IQ signals from different time segments.



Figure 33 IQ Time-Domain Plot and Zoom

## 7.5 PVT

### 7.5.1 Procedure

Click "PvT" in the main settings area and enable "Analyze". Drag the red selection box "PvT-P" in the Max Power vs. Time thumbnail, or adjust the values of "TimeStart" and "TimeLength" to perform power-vs.-time analysis on IQ signals from different time segments.



Figure 34 IQ Power-Time Plot and Zoom

## 7.6 AM Demodulation

As an example, demodulate an AM signal with a carrier frequency of 1 GHz, a power of -20 dBm, a modulation rate of 50 kHz and a modulation depth of 50%.

### 7.6.1 Parameters description

Only some of the important parameters are described here: the important parameters of the AM demodulation section are shown in Table below.

**Table 20 Description of AM Demodulation Parameters**

| AudioFilter |                                                                                                                                          |
|-------------|------------------------------------------------------------------------------------------------------------------------------------------|
| n           | Number of Filter Taps: The larger the number of taps, the steeper the filter's transition band and the smaller the passband ripple.      |
| Fc          | Cutoff Frequency: $0 < F_c < 0.5$ . For example, if set to 0.25, a low-pass filter is applied to half of the bandwidth.                  |
| As          | Stopband Attenuation: The higher the stopband attenuation, the stronger the suppression in the stopband. Attenuation is specified in dB. |
| mu          | Fractional Sample Offset: It is recommended to use the default value.                                                                    |

### 7.6.2 Procedure

1. Set "Center" to 1 GHz. Click the "Trigger" in the main settings area and set the "PreviewTime" to 3 ms;
2. Click "Demod" in the main settings area and set the "Type" in the additional menu to AM;
3. In the Max Power vs. Time thumbnail, drag the edge of the "Spectrum-P" selection box or increase the "TimeLength" in the "FFT" additional menu in the main settings area to expand the analysis range;
4. Click "BW" in the main setting area, and click "Span ▼", to decrease the analysis bandwidth. In this example, set the analysis bandwidth to 768kHz;
5. Click the magnifying glass button "🔍" in the chart setting area, and select the area of interest in the "AM Waveform-P(%)" chart to perform the initial zoom. For PX series tablet instruments, users can further adjust the zoom box size using gestures:
  - Spreading or pinching two fingers horizontally allows for zooming in/out in the horizontal direction
  - Spreading or pinching two fingers vertically allows for zooming in/out in the vertical direction
6. In the current configuration, the AM demodulation interface is shown in the figure below. The displayed content includes the spectrum of the modulated signal, the demodulated time-domain waveform, the audio spectrum, as well as parameters such as AM modulation depth, carrier power, modulation rate, SINAD, signal-to-noise ratio, and total harmonic distortion, allowing users to intuitively assess signal quality.



Figure 35 AM Demodulation

### 7.6.3 Audio analysis

Can be used to test the demodulation sensitivity of an instrument.

1. Refer to [AM demodulation](#) chapter Demodulation of AM signals;
2. Click "Demod" in the main settings area, open "AudioAnalysis" in the submenu, and enable audio analysis. Check whether the audio analysis frequency matches the modulation rate. You can also measure the signal's SINAD and Total Harmonic Distortion.



Figure 36 Audio analysis of AM demodulation

## 7.7 FM Demodulation

As an example, demodulate an FM signal with a carrier frequency of 1 GHz, a power of -20 dBm, a modulation frequency of 5 kHz and a frequency offset of 75 kHz.

### 7.7.1 Parameters description

Please refer to the [AM demodulation parameter description](#) chapter. When listening to FM broadcast signals, the FM demodulated signals can be low-pass filtered to reduce some of the high-frequency noise and make the listening sound purer.

### 7.7.2 Procedure

1. Set "Center" to 1GHz. Click the "Trigger" in the main settings area and set the "PreviewTime" to 3ms;
2. Click "Demod" in the main settings area and set the "Type" in the additional menu to FM;
3. In the Max Power vs. Time thumbnail, drag the edge of the "Spectrum-P" selection box or increase the "TimeLength" in the "FFT" additional menu in the main settings area to expand the analysis range;
4. Click "BW" in the main setting area, and click "Span ▼", to decrease the analysis bandwidth. In this example, set the analysis bandwidth to 384kHz
5. Click the magnifying glass button  in the chart setting area, and select the area of interest in the "FM Waveform-P(%)" chart to perform the initial zoom. For PX series tablet instruments, users can further adjust the zoom box size using gestures:
  - Spreading or pinching two fingers horizontally allows for zooming in/out in the horizontal direction
  - Spreading or pinching two fingers vertically allows for zooming in/out in the vertical direction
6. In the current configuration, the FM demodulation interface is shown in the figure below. The displayed content includes the spectrum of the modulated signal, the demodulated time-domain waveform, the audio spectrum, as well as parameters such as FM modulation frequency offset, carrier power, carrier frequency error, modulation rate, SINAD, signal-to-

noise ratio, and total harmonic distortion, allowing users to intuitively assess signal quality.



Figure 37 FM Demodulation

7.7.3 Audio analysis

After demodulating the FM signal, please refer to the [Audio analysis](#) section for audio analysis of the demodulated signal.

7.8 DDC Digital Down Conversion

Perform digital down conversion and resampling on the IQ data stream to generate sub-IQ streams for further spectrum analysis. The following example demonstrates DDC on a single-tone signal at 1 GHz with a power of -20 dBm.

7.8.1 Parameters description

Only some of the important parameters are described here: some of the important parameters of the DDC digital down conversion are shown in Table below.

Table 21 Description of DDC Digital Down Conversion Parameters

| State      |                                                                                                                               |
|------------|-------------------------------------------------------------------------------------------------------------------------------|
| OffsetFreq | Frequency shift of complex mixing, for >0, the spectrum is shifted to the right; for <0, the spectrum is shifted to the left. |
| Decimate   | Setting the DDC extraction multiplier, i.e., the resampling rate.                                                             |

7.8.2 Procedure

1. Set "Center" to 1 GHz and "Ref. Level" to 0 dBm. Adjust the range of "IQVT-P" in the Max Power vs. Time thumbnail. Select the IQ time-domain plot, click "Graph", and choose "Auto Range" in the Graph submenu;
2. Click "DDC" in the main settings area. In the additional submenu, click "State On" to enable Channel 1. Set DDC1 channel parameters as follows: "Center" = 1.003 GHz, "OffsetFreq" = -3 MHz, "Step" = 1 MHz, and "Decimate" = 3;
3. Click "FFT" in the main settings area. In the additional submenu, select "DDC1" and enable "Analyze". Drag the red selection box "Spectrum-D1" in the Max Power vs. Time thumbnail, or

- adjust "TimeStart" and "TimeLength" to perform spectrum analysis on the IQ sub-stream generated by DDC over different time segments;
- Click "IQvT" in the main settings area. In the additional submenu, select "DDC1" and enable "Analyze". Drag the red selection box "IQvT-D1" in the Max Power vs. Time thumbnail, or adjust "TimeStart" and "TimeLength" to perform spectrum analysis on the IQ sub-stream generated by DDC over different time segments;



Figure 38 View the time-domain diagram of the IQ subflow under DDC

- In the main settings area, click "PvT", select "DDC1", and enable "Analyze". Then drag the red "PvT-D1" box in the Max Power vs. Time thumbnail, or adjust "TimeStart" and "TimeLength" to analyze the IQ sub-stream from DDC over different time segments.



Figure 39 View the power-time graph of the IQ subflow under DDC

## 8. Using of the DET Mode

This chapter describes in detail some of the parameters of the detector analysis mode and the measurement of pulse signals in this mode.

### 8.1 Introduction to the General Parameters of DET Mode

Only some of the important parameters are described here: some of the important parameters of the detector analysis mode are shown in Table 21.

**Table 22 Description of DET Mode Parameters**

| Frequency    |                                                                                                                              |
|--------------|------------------------------------------------------------------------------------------------------------------------------|
| LO Optimize  | Please refer to the parameter with the same name in the <a href="#">Introduction to the General Parameters of SWP Mode</a> . |
| Amplitude    |                                                                                                                              |
| PreAmplifier | Please refer to the parameter with the same name in the <a href="#">Introduction to the General Parameters of SWP Mode</a> . |
| GainStrategy |                                                                                                                              |
| IFGainGrade  |                                                                                                                              |
| Atten        |                                                                                                                              |
| AmpOffset    |                                                                                                                              |
| IFAGC        |                                                                                                                              |
| IFAGCTarget  |                                                                                                                              |
| IFAGCGain    | Unit: dB. Returns the current IF AGC gain; positive values indicate gain, and negative values indicate attenuation.          |
| System       |                                                                                                                              |
| RefCLKSource | Please refer to the parameter with the same name in the <a href="#">Introduction to the General Parameters of SWP Mode</a> . |
| RefCLKOut    |                                                                                                                              |

### 8.2 Pulse Signal Measurement

For example, a pulse modulated signal with a carrier frequency of 1 GHz, a power of -10 dBm, a pulse period of 80 us and a pulse width of 40 us is tested.

#### 8.2.1 Procedure

1. Set "Center" to 1 GHz. Click "Single" in the menu bar to enable single-shot preview mode;
2. Click "Graph" in the chart settings area, then click "Zoom" to enable zoom. Adjust the zoom region by dragging the selected area or by dragging the edges of the zoom box left or right;
3. Select the zoomed plot, click "Graph" in the chart settings area, and choose "Marker Pair" to create two pairs of markers. Move M1R to the rising edge of a pulse, M1D to the falling edge of the same pulse, M2R to the rising edge of the pulse, and M2D to the rising edge of the next pulse. At this point, the values displayed for M1D and M2D in the upper-left corner of the zoomed plot correspond to the pulse width and pulse period, respectively. The duty cycle can be calculated using the following formula:

$$\text{DutyCycle} = \frac{\text{PulseWidth(M1D)}}{\text{PulsePeriod(M2D)}}$$



Figure 40 Pulse Signal Period and Width Measurement

### 8.3 Pulse Signal Detection (Option 72)

If you purchase the Pulse Detection Option at a later date, please refer to the [Pulse Detection Option](#) section to apply for a license in order to use the function properly.

#### 8.3.1 Parameters description

Only some of the important parameters are described here: The important parameters of the pulse signal detection section are shown in Table below.

**Table 23 Description of Pulse Signal Detection Parameters**

| Pulse Det   |                                                                                                                      |
|-------------|----------------------------------------------------------------------------------------------------------------------|
| Threshold   | Pulse detection threshold, greater than the threshold value of the pulse signal will be determined as a valid pulse. |
| Pulse Count | Upper limit of pulse signal detection at current preview time.                                                       |

#### 8.3.2 Procedure

An example is the detection of a pulsed signal at 1 GHz, -20 dBm, with a pulse width of 40 us and a pulse period of 80 us.

1. Set "Center" to 1 GHz and "Ref. Level" to 0 dBm;
2. Click "BW" in the main settings area and adjust the "BW" value in the additional menu to set different analysis bandwidths. In this example, set "AnalysisBW" to 61.44 MHz;
3. Click "Trigger" in the main settings area and set "PreviewTime" to 500  $\mu$ s;
4. Click "Pulse Det" in the main settings area to enable pulse detection. Drag the "Trigger.Level" in the power vs. time plot to set the pulse detection threshold, and adjust "Pulse Count" to set the maximum number of pulses detected within the current preview time;
5. Click "Single" in the menu bar. The pulse detection results under the current configuration are shown in the figure below. From the figure, you can obtain parameters for each detected pulse signal, including Top Level (dBm), Base Level (dBm), Rise Time, Rise Edge, Fall Time,

Fall Edge, Width, PRI, and Duty Cycle. Additionally, statistical parameters of the detected pulses are available, such as Max, Min, and Mean PRI and PW, as well as PRI deviation (%) and PW deviation (%).



Figure 41 Result of Pulse Detection

## 9. Using of the RTA mode

This chapter provides a detailed introduction to certain parameters of the real-time spectrum analysis mode, the disabling of the probability density plot, and the measurement of Wi-Fi signals in this mode.

### 9.1 Introduction to the General Parameters of RTA Mode

Only some of the important parameters are described here: some of the important parameters of the real-time spectrum analysis mode are shown in Table below.

**Table 24 Description of RTA Mode Parameters**

|                 |                                                                                                                                                                                                                               |
|-----------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Frequency       |                                                                                                                                                                                                                               |
| LO Optimize     | Please refer to the parameter with the same name in the <a href="#">Introduction to the General Parameters of SWP Mode</a> .                                                                                                  |
| Amplitude       |                                                                                                                                                                                                                               |
| PreAmplifier    | Please refer to the parameter with the same name in the <a href="#">Introduction to the General Parameters of SWP Mode</a> .                                                                                                  |
| GainStrategy    |                                                                                                                                                                                                                               |
| IFGainGrade     |                                                                                                                                                                                                                               |
| Atten           |                                                                                                                                                                                                                               |
| AmpOffset       |                                                                                                                                                                                                                               |
| IFAGC           |                                                                                                                                                                                                                               |
| IFAGCTarget     |                                                                                                                                                                                                                               |
| IFAGCGain       | Unit: dB. Returns the current IFAGC gain; positive values indicate gain, and negative values indicate attenuation.                                                                                                            |
| Sweep           |                                                                                                                                                                                                                               |
| Acq Time        | Set the data acquisition duration corresponding to a single display update.                                                                                                                                                   |
| SWTMode         | Please refer to the parameter with the same name in the <a href="#">Introduction to the General Parameters of SWP Mode</a> .                                                                                                  |
| Window          |                                                                                                                                                                                                                               |
| Density         |                                                                                                                                                                                                                               |
| Persistence     | <b>Off:</b> Do not retain historical spectrum results; only the current acquisition result is displayed.<br><b>Finite:</b> Historical probability density results are retained for the specified persistence time             |
| Finite Duration | Available when Persistence is set to Finite. Set the retention time for historical probability density results.                                                                                                               |
| Lowest Density  | Set the lower limit of the color mapping for the probability density display.                                                                                                                                                 |
| Highest Density | Sets the upper limit of the color mapping for the probability density display. Decreasing this value enhances color differentiation in lower-density regions, mapping lower-density data to higher levels of the color scale. |

## System

### RefCLKSource

Please refer to the parameter with the same name in the [Introduction to the General Parameters of SWP Mode](#).

### RefCLKOut

## 9.2 Probability Density Plot

The probability density display shows the statistical distribution of the spectrum during continuous acquisition. Different colors indicate the frequency of occurrence at each frequency and amplitude position. A higher frequency of occurrence corresponds to a higher density value and a color closer to the upper end of the current color scale.

### 9.2.1 Parameters description

Click "Graph" in the graph settings area to configure the display parameters for the probability density display.

#### Graph

##### BitMap

On: Enable probability density plot display  
Off: Disable probability density plot display

##### Color

Set the color mapping for the probability density display. Available color scales include Sky, Deep Sea (default), Jet, Cool, Hot, and Grayscale.

##### Afterglow

Adjust the display mapping curve of the probability density display, changing the color and brightness levels for different density regions.

### 9.2.2 Density Display Range

The probability density display uses colors to indicate the frequency of occurrence at different frequency and amplitude positions. The density lower limit and density upper limit define the mapping range between density values and the color scale.

Decreasing the density upper limit maps lower density values to higher levels of the color scale, enhancing color differentiation between low-density regions. If the density upper limit is set too low, higher-density regions may be concentrated at the upper end of the color scale.

### 9.2.3 Persistence Settings

When "Persistence" under "Density" is set to "Off", only the current probability density result is displayed. When set to "Finite", historical probability density results are retained for the specified persistence time. Increasing the persistence time appropriately makes it easier to observe intermittent or short-duration signals.

Note: "Afterglow" under Graph adjusts the display mapping effect of the probability density display. "Persistence" and "Finite Duration" under Density determine how historical probability density results are retained and for how long.

### 9.2.4 Close Probability Density Plot

Click Graph in the chart settings area, and in the pop-up window disable "BitMap" to turn off the probability density plot.



Figure 42 Close Probability Density Plot

### 9.3 WIFI Signal Measurement

The following example uses a 2.4 GHz Wi-Fi signal to demonstrate the basic use of the probability density display in Real-Time Spectrum Analysis mode.

1. Connect the antenna to the "RFIN" RF input port;
2. Set "Center" to 2.44 GHz and select an appropriate color scale according to the actual signal conditions;
3. Adjust the Afterglow under Graph according to the display effect so that different density regions have clearly distinguishable color levels;
4. To observe intermittent Wi-Fi signals, set "Persistence" under "Density" to "Finite" and configure an appropriate persistence time to retain historical probability density results for a specified period;
5. Adjust the density upper and lower limits as needed so that signals with different frequencies of occurrence can be clearly distinguished by color;
6. Observe the frequency distribution and density variations of the Wi-Fi signal in the probability density display.

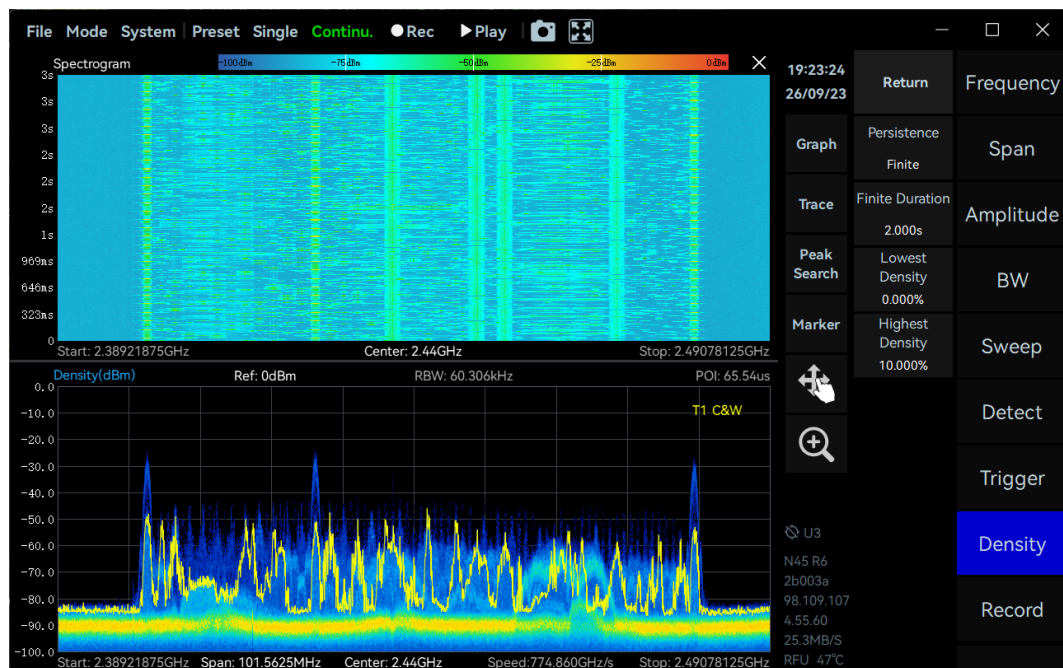


Figure 43 Probability Density Display of a Wi-Fi Signal

## 10. Digital Demodulation (Option 71)

If you purchase the Pulse Detection option at a later date, please refer to the [Digital Demodulation option](#) section to apply for a license and a demodulation library in order to use the function properly.

### 10.1 Parameters description

Only some of the important parameters are described here: some of the important parameters are shown in Table below.

**Table 25 Description of Digital Demodulation Parameters**

| Digital Demod         |                                                                                                                                                                                                                                                            |
|-----------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>SymbolRate</b>     | The number of symbols per second transmitted by the signal, which should be filled in according to the symbol rate of the modulated signal to ensure correct demodulation at the receiving end                                                             |
| <b>ModType</b>        | 2ASK, 2FSK, 4FSK, GMSK, BPSK, QPSK, 8PSK, 16QAM, 32QAM, 64QAM, 128QAM, 256QAM                                                                                                                                                                              |
| <b>FilterAlpha</b>    | The roll-off rate of the filter used to limit the signal bandwidth in the transition band needs to be consistent with the roll-off coefficient at the transmitter to ensure efficient processing and correct demodulation of the signal by the demodulator |
| <b>Average number</b> | Increasing the number of averages reduces jitter in parameters such as EVMs                                                                                                                                                                                |

### 10.2 Function Overview

The initial interface of the digital demodulation mode consists of the modulated signal spectrogram, the demodulated constellation diagram, the eye diagram, and the demodulation parameters, including: error vector magnitude (EVM), magnitude error, phase error, frequency error, signal-to-noise ratio (SNR/MER), and a partially decoded bit sequence. The modulation quality of the signal is analyzed in depth, providing several error indicators to effectively assess the integrity and reliability of the signal in transmission.

### 10.3 Procedure

As an example, demodulation of a 64QAM signal at 1 GHz, -20 dBm, SymbolRate 1 MHz, FilterAlpha 0.35.

1. Click "Mode" -> "Digital Demod";
2. Set the "Center" to 1 GHz and the "Ref.Level" to 0 dBm;
3. Click "Demod" in the main setting area, set "ModType" to QAM64, "SymbolRate" to 1 MSPS, "FilterType" to 0.35, and "Average Count" to 10 in the additional menu, then click "Single" in the menu bar. MSPS, "FilterType" is set to 0.35, "Average Count" is set to 10, click "Single" in the menu bar, the demodulation result under the current configuration is shown in the figure below. The demodulation result under the current configuration is shown in the figure below.

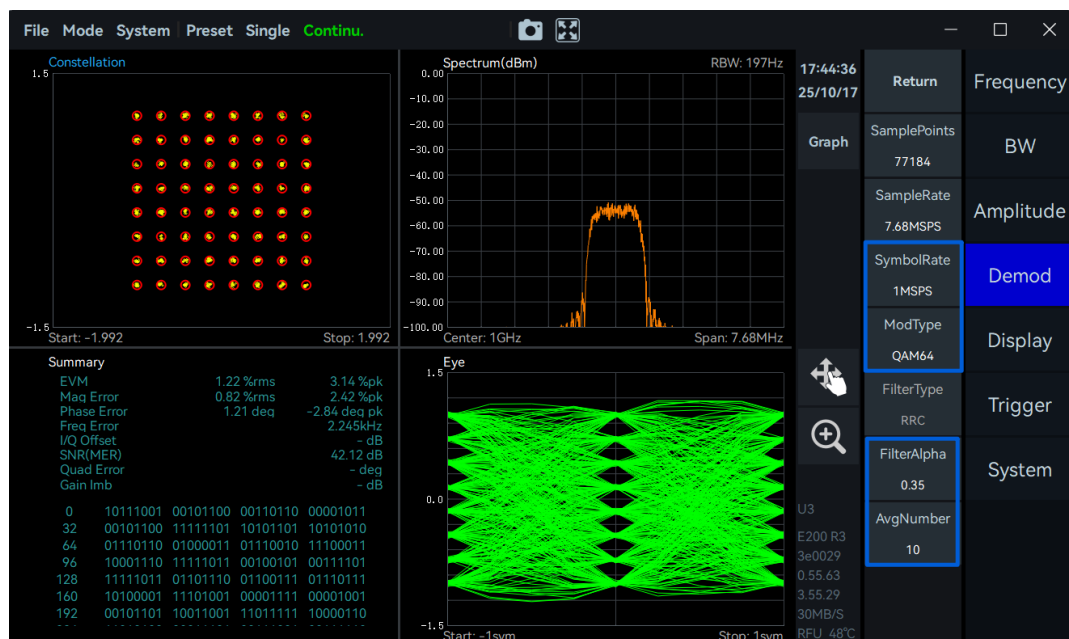


Figure 44 64QAM Demodulation

# 11. Harmonic Analysis Mode

## 11.1 Version Requirements

1. Refer to the [Viewing Instrument Information](#) section to view the soft and firmware version;
2. Ensure the version meets the following requirements:
  - GUI Version: 4.3.55.24 or above
  - API Version: 0.55.0 or above
  - FPGA Version: 0.55.0 or above
  - MCU Version: 0.55.0 or above
3. If the GUI version does not meet the above requirements, please refer to the section on [Software and Firmware Update](#) to obtain the appropriate version of the host computer software.

## 11.2 Enable Harmonic Analysis Function

After updating the software and firmware to the required version, restart the host software, and click "Mode" -> "Harmonics" in the menu bar to use the harmonic analysis function normally.

## 11.3 Parameters description

Only some of the important parameters are described here: the important parameters of the harmonic analysis section are shown in Table below.

**Table 26 Description of Harmonic Analysis Parameters**

| Frequency   |                                                                                                                                                                                                              |
|-------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Center      | The center frequency of the fundamental signal.                                                                                                                                                              |
| Span        |                                                                                                                                                                                                              |
| Span        | The measurement bandwidth for each harmonic. Range: 10 Hz to 100 MHz.                                                                                                                                        |
| Amplitude   |                                                                                                                                                                                                              |
| Offset      | Adjust the position of the spectrum plot along the amplitude axis.                                                                                                                                           |
| Meas        |                                                                                                                                                                                                              |
| Harm Count  | Set the number of harmonics to measure and plot, up to 10.                                                                                                                                                   |
| Meas Type   | Peak: Measure the peak power of the fundamental and each harmonic.<br>ChannelPower: Measure the channel power of the fundamental and harmonics within their respective sweep bandwidths.                     |
| Trace Type  | ClearWrite: Update the spectrum plot in real time, suitable for observing instantaneous signal changes.<br>MaxHold: Hold the peak value of the displayed signal, suitable for capturing instantaneous peaks. |
| PK Tracking | On: Enable peak tracking of the fundamental signal, aligning its peak to the center frequency.                                                                                                               |
| THD         | Used to evaluate the distortion level of the signal.                                                                                                                                                         |

## 11.4 Procedure

An example is the measurement of the third harmonic of a 1 GHz, -20 dBm signal.

1. Click "Frequency" in the main settings area and set "Center" to 1 GHz;
2. Click "Amplitude" and set "Ref. Level" to -10 dBm;
3. Click "Meas", set "Harm Count" to 3, and enable "PK Tracking". Keep other parameters at their default values;
4. Click "Span" and set the "Span" to 10 MHz;
5. Click "BW" and adjust "RBW" and "VBW" values to stabilize the trace. In this example, set RBW to 1 kHz and VBW to 100 Hz;
6. The test results are shown in the figure below. The THD is displayed in the top-right corner of the spectrum plot. In the harmonic measurement table below, the frequencies, amplitudes, and differences from the fundamental of the second and third harmonics are listed.

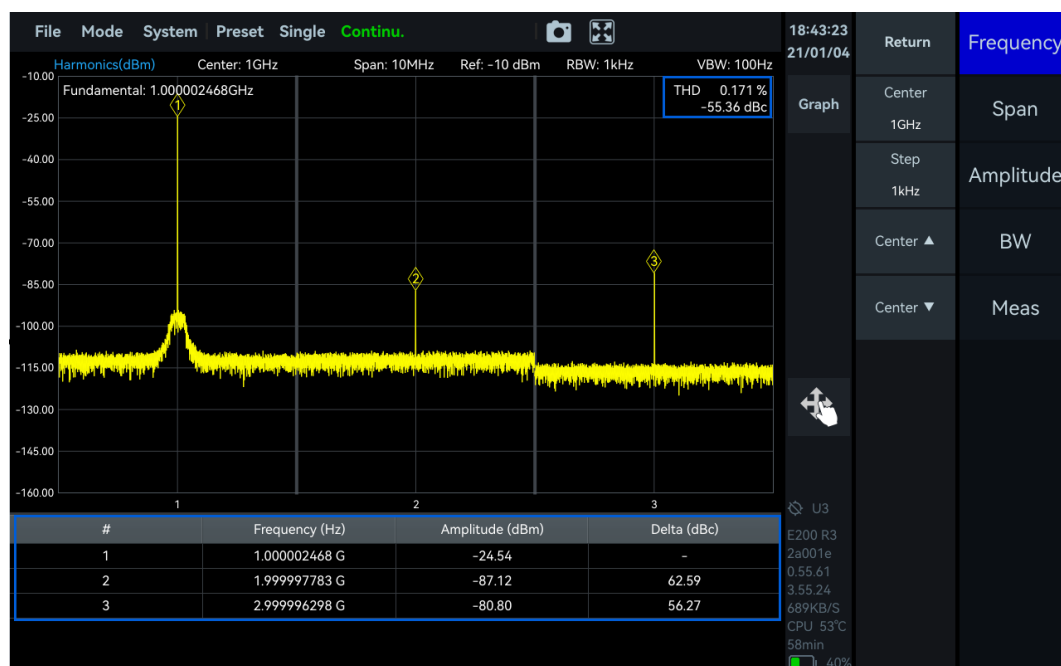


Figure 45 Measurement of Third Harmonic

## 12. Phase Noise Measurement Mode

### 12.1 Version Requirements

1. Refer to the [Viewing Instrument Information](#) section to view the soft and firmware version;
2. Ensure the version meets the following requirements:
  - GUI Version: 4.3.55.12 or above
  - API Version: 0.55.58 or above
  - FPGA Version: 0.55.17 or above
  - MCU Version: 0.55.49 or above
3. If the soft and firmware version does not meet the above requirements, please refer to the section on [Software and Firmware Update](#) to update.

### 12.2 Enable Phase Noise Measurement Function

After updating the software and firmware to the required version, restart the host software, and click "Mode" -> "Phase Noise" in the menu bar to use the phase noise measurement function normally.

### 12.3 Parameters description

Only some of the important parameters are described here: The important parameters for the phase noise measurement are shown in Table below.

**Table 27 Description of Phase Noise Measurement Parameters**

| Frequency     |                                                                                                                                                                                                                                                |
|---------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Center        | Set the center frequency of the fundamental.                                                                                                                                                                                                   |
| Start Offset  | Set the frequency offset start point: Range: 1 Hz to 9 MHz.                                                                                                                                                                                    |
| Stop Offset   | Set the frequency offset stop point: Range: 10 Hz to 10 MHz.                                                                                                                                                                                   |
| Threshold     | Set the threshold above which carriers will be identified.                                                                                                                                                                                     |
| Meas          |                                                                                                                                                                                                                                                |
| RBW/Offset    | RBW Ratio: (RBW of each frequency segment or start frequency of each frequency segment), range: 0.01 to 0.3.                                                                                                                                   |
| Detect        | Frame Detection Rate: The default configuration is recommended. If the test signal exhibits significant low-frequency jitter near the carrier, increase the frame detection rate in the near region to obtain more stable measurement results. |
| Trace         |                                                                                                                                                                                                                                                |
| Average       | Set the number of averaging times for the trace.                                                                                                                                                                                               |
| Smooth        | On: Enable trace smoothing.<br>Off: Disable trace smoothing.                                                                                                                                                                                   |
| Window Length | Set the window length of the smoothing algorithm, range: 0 to 10%.                                                                                                                                                                             |

## 12.4 Procedure

### 12.4.1 Phase Noise Measurement with Known Carrier Information

As an example, the phase noise of a 1 GHz, 0 dBm signal is measured over an offset range of 100 Hz to 10 MHz.

1. Click "Frequency" in the main settings area. In the additional menu, set "Center" to 1 GHz, "Start Offset" to 100 Hz, and "Stop Offset" to 10 MHz. It is recommended to keep the other parameters at their default settings;
2. If the test signal exhibits strong jitter near the carrier, click "Meas" in the main settings area. Then, in the additional menu, select "Detect". In the pop-up window, appropriately increase the frame detection rate for the corresponding frequency band to obtain more convergent measurement results;

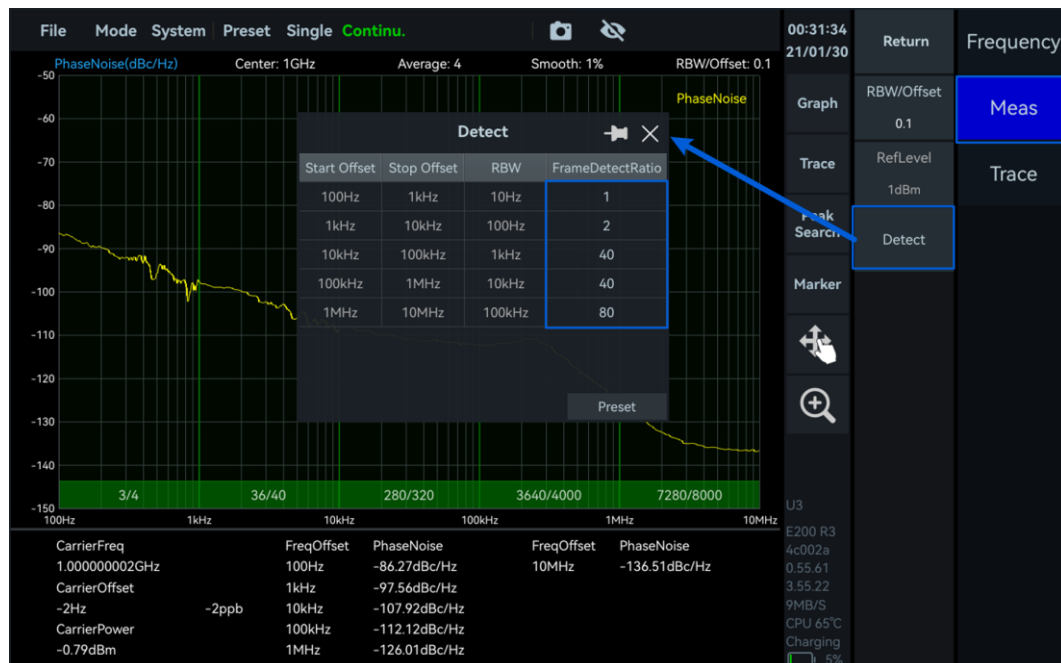


Figure 46 Pulse Signal Detection Settings

3. If significant spurious components appear in the single-sideband phase noise spectrum, click "Trace" in the main settings area. Then, in the additional menu, select "Window Length" and gradually increase its parameter value to reduce the impact of spurious signals on the measurement results;
4. The instrument will automatically perform phase noise measurements within the specified frequency offset range. The measurement results are shown below. In the phase noise measurement table at the bottom of the interface, information about the carrier as well as the phase noise values (dBc/Hz) at characteristic offset points can be obtained.



Figure 47 Result of Phase Noise Measurement

#### 12.4.2 Phase Noise Measurement with Unknown Carrier Information

When the signal carrier parameters are unknown, it is recommended to follow the procedure below for phase noise measurement

1. Click "Carrier". The instrument will automatically perform a full-band scan to search for and locate peak signals that exceed the carrier threshold, which will be used as the test carrier;
2. After locating the carrier signal, refer to the [Phase Noise Measurement with Known Carrier Information](#) to set the start and stop frequency offsets, and perform the phase noise measurement.

## 13. Signal/Tracking Generator Function (Option 60 61 62)

The built-in signal/tracking generator option can output single-tone signals, frequency sweep signals, and power sweep signals, and supports tracking generator functionality. This option is only available for all-new PXN series.

**Table 28 Description of AUXS Mode Parameters**

|                            |                                                                                                                                                      |
|----------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>RF Out</b>              | On: Enables the signal source output<br>Off: Disables the signal source output                                                                       |
| <b>Mode</b>                | Fixed Frequency mode, frequency sweep, power sweep, TG                                                                                               |
| <b>FixedPoint</b>          |                                                                                                                                                      |
| <b>Center</b>              | Set the frequency for single-tone signals                                                                                                            |
| <b>Level</b>               | Set power for single-tone signals                                                                                                                    |
| <b>FreqSweep</b>           |                                                                                                                                                      |
| <b>Start</b>               | Set the start frequency of the frequency sweep signal                                                                                                |
| <b>Stop</b>                | Set the stop frequency of the frequency sweep signal                                                                                                 |
| <b>Step</b>                | Set the frequency step of the frequency sweep signal                                                                                                 |
| <b>Dwell Time</b>          | Set the dwell time of the frequency sweep signal                                                                                                     |
| <b>PowerSweep</b>          |                                                                                                                                                      |
| <b>Center</b>              | Set the output signal center frequency                                                                                                               |
| <b>Start</b>               | Set the start power of the power sweep signal                                                                                                        |
| <b>Stop</b>                | Set the stop power of the power sweep signal                                                                                                         |
| <b>Step</b>                | Set the power step of the power sweep signal                                                                                                         |
| <b>DwellTime</b>           | Set the dwell time for sweep signals, effective in "PowerSweep" and "FrequencySweep" modes                                                           |
| <b>TG</b>                  |                                                                                                                                                      |
| <b>Output Power</b>        | Set the amplitude of the tracking generator output signal.                                                                                           |
| <b>RBW</b>                 | Set the resolution bandwidth, which affects the measurement noise floor and sweep speed.                                                             |
| <b>Through Calibration</b> | Save the current measurement trace as the reference baseline and enable normalization.                                                               |
| <b>Normalize</b>           | Perform normalization based on the reference trace to eliminate system path loss, displaying only the frequency response characteristics of the DUT. |
| <b>Show Reference</b>      | Display the saved reference trace for comparison and analysis.                                                                                       |

### 13.1 Instructions for Using the ASG Function

The signal is output through the instrument's RFOUT port, which can either provide an input signal to other devices or be connected via cable to the instrument's own RF input port. The following example demonstrates a self-transmit-and-receive setup.

#### 13.1.1 Output a Single-Tone Signal

1. Click "AUXS" -> "RF On" in the main settings area to enable the signal source option;
2. In the "AUXS" submenu, set "Center" to 1 GHz and "Level" to -20 dBm to output a single-tone signal at 1 GHz with a power level of -20 dBm.

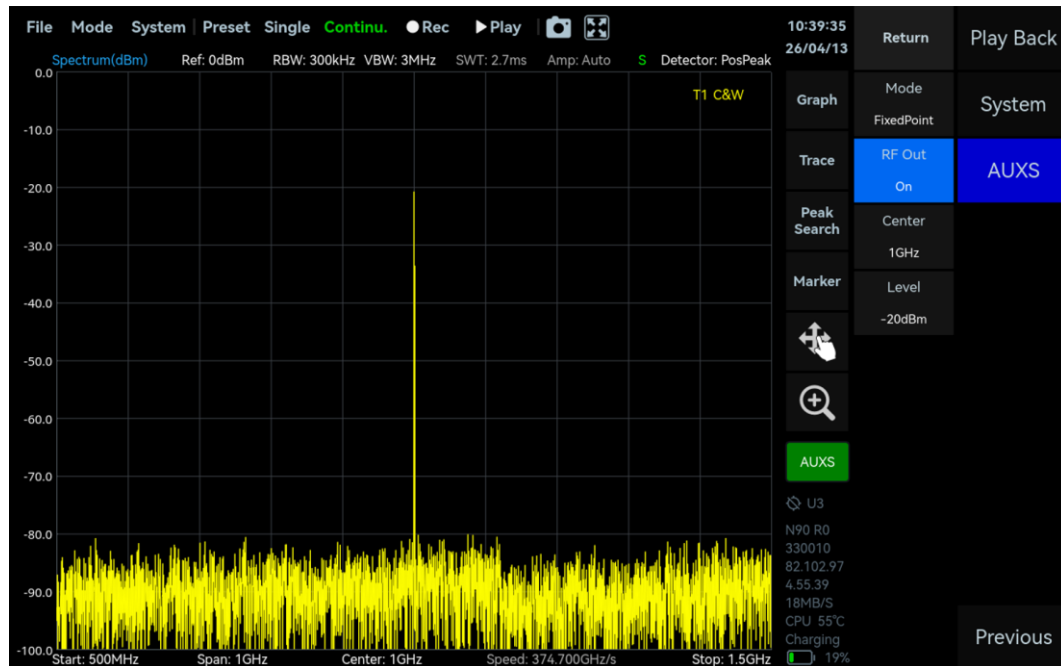


Figure 48 AUXS Single-Tone Signal Output

#### 13.1.2 Output a Frequency Sweep Signal

1. Click "AUXS" in the main setting area, set the "Mode" to Frequency Sweep, and enable "RF Output";
2. In the sweep signal parameter settings area, set Output Power to -20 dBm, Start Frequency to 3 GHz, Stop Frequency to 3.5 GHz, Frequency Step to 40 MHz, and Dwell Time to 8 ms;
3. The built-in signal generator outputs a frequency sweep signal with a start frequency of 3 GHz, a stop frequency of 3.5 GHz, a frequency step of 40 MHz, a dwell time of 8 ms, and an amplitude of -20 dBm.

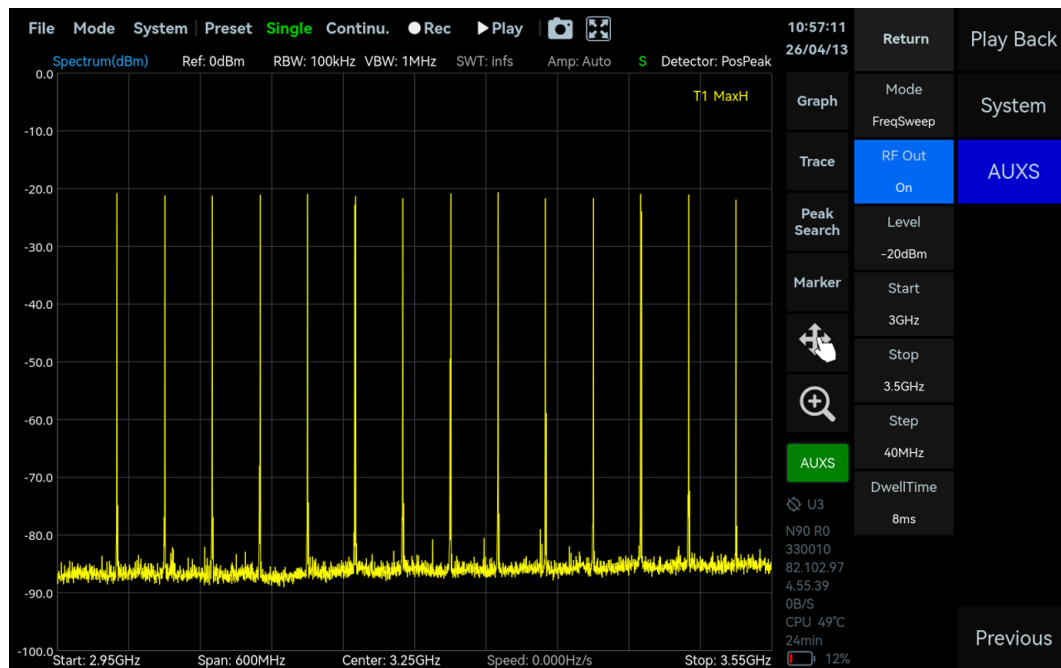


Figure 49 AUXS Frequency Sweep Signal Output

### 13.1.3 Output a Power Sweep Signal

1. Click "AUXS" in the main settings area, set the "Mode" to Power Sweep, and enable "RF Output";
2. In the power sweep signal parameter settings area, set "Center Frequency" to 1 GHz, "Start Power" to -40 dBm, "Stop Power" to -10 dBm, "Power Step" to 1 dBm, and "Dwell Time" to 100 ms;
3. The built-in signal generator outputs a power sweep signal with a frequency of 1 GHz, a start power of -40 dBm, a stop power of -10 dBm, a power step of 1 dBm, and a dwell time of 100 ms.

### 13.1.4 Tracking Generator (TG)

The tracking generator (TG) is a core function of a spectrum analyzer used for measuring the frequency response of devices under test (DUT). When the TG function is enabled, the RF output port of the spectrum analyzer generates a signal that is strictly synchronized with the current sweep frequency.

1. Set the instrument's "Center Frequency" and "Span" according to the operating frequency band of the device under test (DUT);
2. Click "AUXS" → "RF On" in the main settings area, select "TG" as the mode to enable the tracking generator, and set an appropriate "Output Power" according to the DUT characteristics;
3. Use a high-quality RF coaxial cable to directly connect the spectrum analyzer's TG output port to the RF input port;
4. After the trace on the screen becomes stable, press the "Through Calibration" button to save the measurement curve that includes system cable loss, and enable the normalization function to eliminate system errors from the cable and instrument (after normalization, the trace typically appears as a near 0 dB flat line);

5. Disconnect the through connection and insert the DUT between the TG output port and the RF input port. The trace displayed on the screen now represents the true frequency response of the DUT.

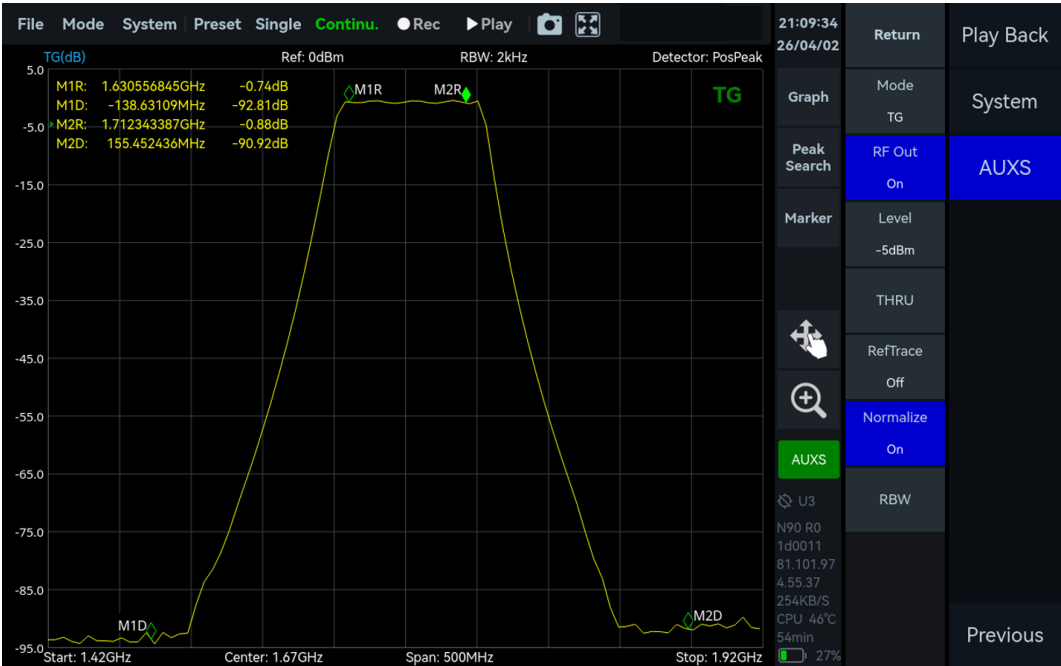


Figure 50 Frequency response curve of a band-pass filter

## 14. EMI Pre-Compliance Measurements (Option 74)

If you purchase the EMI Pre-Compliance Measurements Option at a later date, please refer to the [EMI Pre-Compliance Measurements Option](#) section to apply for the corresponding license before using this feature.

### 14.1 Version Requirements

Refer to the [Viewing Instrument Information](#) section to check the instrument software and firmware versions. For all instruments, ensure that the GUI version is 4.4.55.52 or later.

### 14.2 Introduction to EMI Pre-Compliance Measurements

EMI pre-compliance measurements are used for preliminary evaluation of electromagnetic compatibility performance during the product development stage. It is primarily used to analyze electromagnetic interference (EMI) emissions, helping engineers quickly identify potential sources of interference. The mode supports both standard test templates and custom test configurations, allowing users to configure parameters such as the scan frequency range, RBW, dwell time, detector type, and limit lines. The complete test workflow consists of the following three stages:

1. **Scan:** Automatically performs high-speed frequency sweeps based on the configured scan table to acquire spectrum data.
2. **Search:** Automatically identifies frequencies that approach or exceed the configured limit line based on the specified search margin, and extracts these candidate interference frequencies into the signal list.
3. **Measure:** Performs fixed-frequency dwell measurements on each frequency in the signal list and uses Peak, Quasi-Peak (QP), RMS, and Average (Avg) detectors to obtain accurate compliance measurement results.

### 14.3 Introduction to EMI Pre-Compliance Mode Interface

In EMI Pre-Compliance mode, the main interface is divided into the following five functional areas:



figure 51 EMI Pre-Compliance Mode Interface introduction

- Spectrum Display Area:** Displays spectrum traces and limit lines within the current scanned frequency band. It supports the overlay display of multiple limit lines, including Peak, QP, RMS, and Avg.
- Measurement Display Area:** During the precision measurement phase, this area refreshes in real time to display the fixed-point dwell measurement values of the current target frequency point, providing data for four detector types:
  - **Peak:** The maximum amplitude value of the signal acquired within the measurement time, used to quickly capture transient or intermittent interference signals.
  - **QP (Quasi-Peak):** Utilizes the quasi-peak detection method defined in CISPR 16-1-1. It weights the signal within the measurement time based on specified charge and discharge time constants, used to evaluate the level of repetitive electromagnetic disturbances.
  - **RMS (Root Mean Square):** Calculates the root-mean-square value of the acquired signal within the measurement time to reflect the effective power level of the signal. It is commonly used for broadband noise and random disturbance evaluation.
  - **Avg (Average):** Calculates the average value of the acquired signal within the measurement time, used to evaluate the average amplitude level of continuous wave (CW) or stable repetitive disturbance signals.
- Scan Table:** Used to configure and manage the scan frequency bands for EMI pre-compliance measurements. The instrument performs scans sequentially according to the frequency bands configured in the table, providing spectrum data for subsequent signal searches.
- Signal Table:** Used to store, manage, and display interference frequency points pending precision measurement as well as those already measured. After the instrument completes a scan, the software automatically extracts and adds the compliant disturbance frequency points to the signal table based on the configured search mode, search margin, and limit conditions. During continuous scanning, the software deduplicates and updates the

frequency points in the table according to the following logic:

- **Deduplication and Replacement:** If the frequency interval between a newly searched signal and an existing signal in the signal table is smaller than the current measurement RBW, the software determines them to be the same interference signal. In this case, the latest searched frequency point and its data are retained, automatically overwriting the previously searched frequency point information.
- **Append and Retain:** If the frequency interval between the new signal and all existing signals in the list is greater than or equal to the current measurement RBW, the software determines it to be an independent new interference source and automatically appends it to the list as a new entry.

In the subsequent precision measurement phase, the instrument sequentially performs fixed-point dwell measurements on each frequency point, filling the measured values (such as Peak, QP, RMS, and Avg) into the corresponding data rows in real time.

5. **Measurement Parameter Settings Area:** Used to configure parameters during the EMI pre-compliance measurements process, such as amplitude control, search modes, and the linkage logic between scanning and precision measurement. For detailed descriptions, please refer to the chapter on [introduction to General Parameters for EMI Pre-Compliance](#).

#### 14.4 Introduction to General Parameters for EMI Pre-Compliance

**Table 29 Description of Parameters in the Measurement Parameter Settings Area**

| ScanTable   |                                                                                                                                                                                                                                                                                                                 |
|-------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| SelectStd.  | Imports predefined scan configuration files to quickly load scan frequency bands and related settings.                                                                                                                                                                                                          |
| SaveStd.    | Exports the current scan configuration for convenient reuse in the future.                                                                                                                                                                                                                                      |
| AddBand     | Adds a new scan frequency band to the scan table.                                                                                                                                                                                                                                                               |
| DeleteBand  | Deletes the selected scan frequency band from the scan table.                                                                                                                                                                                                                                                   |
| Amplitude   |                                                                                                                                                                                                                                                                                                                 |
| Units       | Sets the amplitude display unit, including dBm, dBmV, and dBuV.                                                                                                                                                                                                                                                 |
| AF          | Refer to the <a href="#">description of antenna factor parameter</a> table to import or edit the antenna factors corresponding to different frequency points. The software compensates the measurement results based on the current measurement frequency and displays the corresponding field strength values. |
| Meas        |                                                                                                                                                                                                                                                                                                                 |
| Search Mode | <p>Sets the signal search method.</p> <p>Spurious: Searches for interference signals approaching or exceeding the limit based on the limit line and margin.</p> <p>Peak: Searches for signals with prominent amplitudes based on spectrum peak characteristics.</p>                                             |
| Margin      | <p>Sets the search margin to adjust the signal search threshold. A lower margin lowers the search threshold and increases signal search sensitivity; a higher margin reduces the number of searched signals.</p> <p>Range: -20 dB to 20 dB</p>                                                                  |

|                            |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                         |
|----------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Meas Time</b>           | Configures the measurement time for a single signal frequency point. Within this duration, the instrument continuously acquires data for the current frequency point and calculates Peak, QP, RMS, and Avg measurement values based on the acquired results.<br>Range: 0.1 s to 10 s                                                                                                                                                                                                                                                    |
| <b>Sequence</b>            | Sets the execution workflow for EMI pre-compliance measurements:<br>Scan & Search: Executes the scan and signal search workflow, automatically adding signals that meet the search conditions to the target signal table.<br>Measure: Sequentially measures the frequency points in the signal list and updates the corresponding measurement results.<br>Scan, Search & Measure: Executes the complete EMI pre-compliance measurements workflow; the instrument sequentially performs scanning, signal search, and signal measurement. |
| <b>SignalTable</b>         |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                         |
| <b>Measure SignalTable</b> | During Scan and Search mode, press this key to pause the current scan and prioritize point-by-point measurements of the signals under test that have already been detected and listed in the scan table. After the measurements are completed, the instrument automatically resumes the previously interrupted scan and search operation.                                                                                                                                                                                               |
| <b>Measure ThisPoint</b>   | Clicking this pauses the current operation to perform continuous measurement on the currently selected frequency point, refreshing Peak, QP, RMS, and Avg measurement results in real time. Clicking it again stops the measurement and resumes the original workflow.                                                                                                                                                                                                                                                                  |
| <b>AddToList</b>           | Manually adds a target signal of a specified frequency to the signal table.                                                                                                                                                                                                                                                                                                                                                                                                                                                             |
| <b>ExportList</b>          | Exports the frequency point information and corresponding measurement results from the current signal table.                                                                                                                                                                                                                                                                                                                                                                                                                            |
| <b>TransFactor</b>         | Used to compensate for the amplitude of the received signal, typically consisting of the antenna factor and cable loss.                                                                                                                                                                                                                                                                                                                                                                                                                 |

## 14.5 Operating Steps

This section uses the import of the FCC Part 15, RAD, Class B (3m) template as an example to demonstrate the complete workflow, from standard loading and automatic parameter configuration to signal search and precision measurement.

### 1. Configure the Scan Table

- 1) Click "Mode" -> "EMI Pre-Compliance" to enter the EMI pre-compliance mode;
- 2) Click "[Scantable](#)" -> "SelectStd." in the parameter settings area, select FCC Part 15, RAD, Class B (3m) from the pre-stored standards list, and click confirm.

Note: Users can also manually edit custom scan frequency bands using "AddBand" or "Delete Band", allowing flexible adjustments to the configuration parameters for each band (including start frequency, stop frequency, RBW, dwell time, detector type, and limit lines).

### 2. Configure Amplitude and Antenna Factor

- 1) Click "[Amplitude](#)" -> "Ref.Level" and adjust the reference level and measurement unit as needed. In this example, the default value of 107 dBuV is used;
- 2) If a receiving antenna is used, refer to the [description of antenna factor parameter](#) table to import the corresponding antenna factor for data compensation, which converts the display unit into a field strength unit.

### 3. Configure the Search and Measurement Workflow

Click "Meas", set "Search Mode" to Spurious, "Margin" to -10 dB, keep "TimeMode" on Auto, and set "Sequence" to Scan and Search.

### 4. Execute the Test and View/Export Results

- 1) According to the above configuration and execution strategy, the instrument sequentially performs "scan" -> "search", and automatically extracts and adds compliant disturbance frequency points to the signal table;
- 2) Click "SignalTable" -> "Measure SignalTable". The system will pause the scan and search operation, sequentially perform fixed-point dwell measurements on each frequency point in the signal table based on the set measurement time, and display the precision measurement results (such as Peak, QP, RMS, and Avg) in real time;
- 3) Enter the "Frequency" and "Bandwidth" in the setting fields, and click "AddToList" to manually add a specific frequency point to the signal table. Click "MeasureThisPoint" to continuously measure and refresh the data at the selected frequency point;
- 4) After the measurement is complete, click "ExportList" to export and save the current signal list and the corresponding precision measurement data in CSV format to the "/reports" folder.

Note: **Automatic Resume:** After the precision measurement of all frequency points in the signal table is completed, the system will automatically resume the previously configured "Sequence".

**Manual Interruption:** If Stop Measure is clicked during the precision measurement process, the system will immediately terminate the current precision measurement task and return directly to the previously configured "Sequence".



figure 52 EMI Pre-Compliance Measurements Diagram

## 15. Additional Functions

This chapter briefly describes the IF outputs of the instrument, as well as the trigger function, the input of an external reference clock, and the remote control of the device.

### 15.1 Description of Trigger Functions

#### 15.1.1 SWP Frequency Sweep Mode

| Trigger       |                                                                                                                                                                                                           |
|---------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| TriggerSource | FreeRun, Ext.PerHop, Ext. PerSweep, Ext.PerProfile, InXpps.PerHop, InXpps.PerSweep, InXpps.PerProfile                                                                                                     |
| TriggerEdge   | RisingEdge, FallingEdge, DoubleEdge                                                                                                                                                                       |
| TriggerOut    | None.<br>PerHop: outputs a trigger for each completed frame of analysis.<br>PerSweep: outputs a trigger for each trace scan completed.<br>PerProfile: outputs a trigger for each switching configuration. |
| PulsePolarity | Positive, Negative                                                                                                                                                                                        |

#### 15.1.2 Fixed Frequency Point Mode for IQS, DET and RTA

| Trigger             |                                                                                                                                                                                                                                                                                                                                                                                                                 |
|---------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| TriggerSource       | External, Bus, Level, Timer, DevSyncByExt, DevSyncBy1PPS, GNSS1PPS                                                                                                                                                                                                                                                                                                                                              |
| TriggerEdge         | RisingEdge, FallingEdge, DoubleEdge                                                                                                                                                                                                                                                                                                                                                                             |
| TriggerDelay        | Set the time to delay acquisition after triggering                                                                                                                                                                                                                                                                                                                                                              |
| PreTrigger          | Set the time to collect in advance before triggering                                                                                                                                                                                                                                                                                                                                                            |
| ReTrigger           | The instrument responds multiple times after capturing a trigger                                                                                                                                                                                                                                                                                                                                                |
| ReTrigger-On        |                                                                                                                                                                                                                                                                                                                                                                                                                 |
| Count               | After a single trigger response, additional responses may be required.                                                                                                                                                                                                                                                                                                                                          |
| Period              | The time interval between multiple responses to a single trigger corresponds to the trigger period under the timer trigger mode.                                                                                                                                                                                                                                                                                |
| TriggerSource-Level |                                                                                                                                                                                                                                                                                                                                                                                                                 |
| Level               | Set the level trigger threshold. A signal exceeding the threshold indicates that the trigger condition is met.                                                                                                                                                                                                                                                                                                  |
| SafeTime            | Set the debounce safety time for the level trigger.                                                                                                                                                                                                                                                                                                                                                             |
| TriggerSource-Timer |                                                                                                                                                                                                                                                                                                                                                                                                                 |
| Period              | Trigger period under the timer trigger mode                                                                                                                                                                                                                                                                                                                                                                     |
| Sync                | Not synchronized with the external trigger<br>Synchronized with the external trigger's rising edge<br>Synchronized with the external trigger's falling edge<br>Single-shot synchronization with the external trigger's rising edge<br>Single-shot synchronization with the external trigger's falling edge<br>Synchronization with the GNSS-1PPS rising edge<br>Synchronization with the GNSS-1PPS falling edge |

Single-shot synchronization with the GNSS-1PPS rising edge  
 Single-shot synchronization with the GNSS-1PPS falling edge

## 15.2 IF Output Application Guide

The frequency of the analog IF output signal is between  $312.5 \text{ MHz} \pm 50 \text{ MHz}$ . The center frequency of the analog IF output of each instrument can be viewed in the IF calibration file in the "/bin/CalFile" folder in the software installation directory.

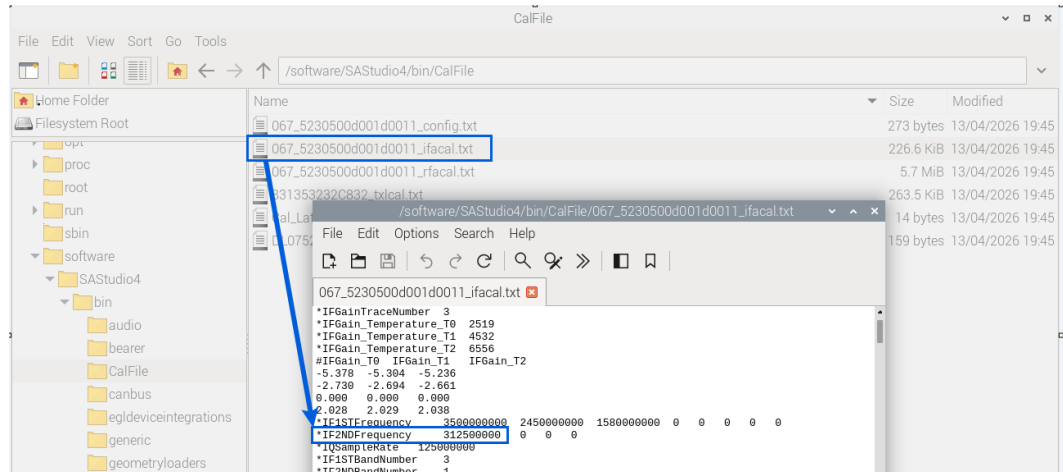


Figure 53 Check the IF Output Center Frequency on PXN Series Instruments

## 15.3 External Reference Clock Input

1. Refer to the interface description in the *Quick Start Guide* to input the external reference clock;
2. In the main settings area, click "Next" -> "System", set the reference clock frequency "RefCLKFreq" to 10 MHz, and select "External" as the reference clock source "RefCLKSource". If the reference clock source displays "External", the switch is successful. If it reverts to "Internal" and an error message pops up, the switch has failed. In this case, click "Preset" to switch back to the internal clock.

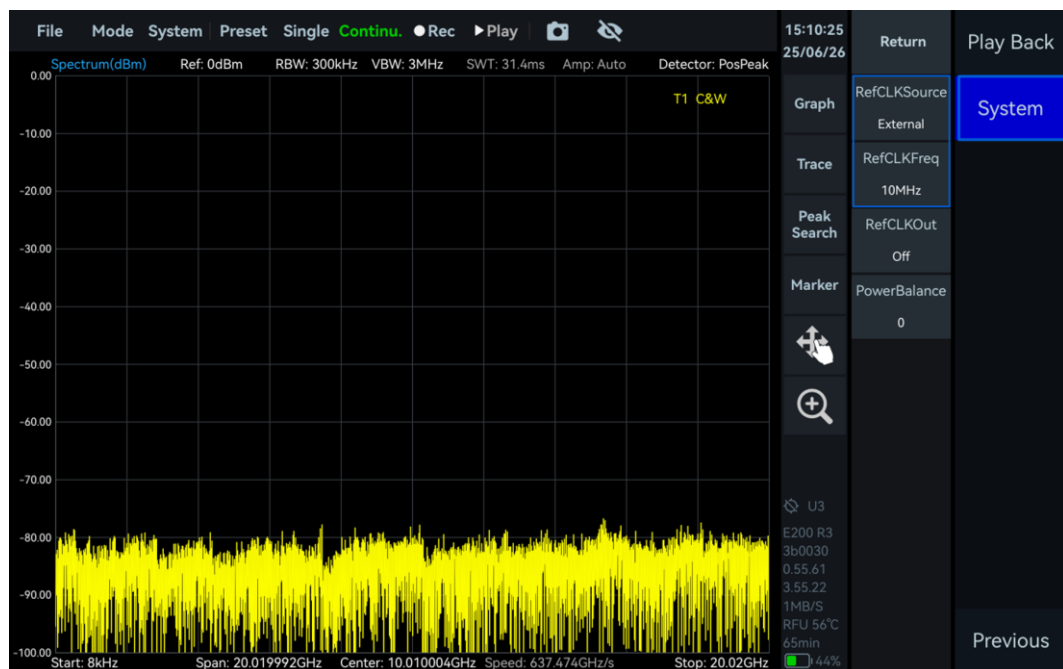


Figure 54 Use an external 10 MHz reference clock

## 15.4 Connecting and Operating Multiple Instruments Simultaneously

A single window of the software can only control one instrument. To operate multiple instruments simultaneously, you can open multiple windows within the same software, with each window corresponding to a different instrument number.

This section takes the simultaneous operation of two SA series instruments as an example. The specific steps are as follows:

1. Correctly connect the two instruments to the host computer;
2. Copy the calibration files corresponding to the two instruments into the "/bin/CalFile" folder in the software directory;
3. Double-click the executable program in the "bin" folder to open the software and enable the instrument with device number 0;
4. Go to the "configuration" folder in the software directory, open the "Setting.ini" text file, and change "DeviceNum=0" to "DeviceNum=1";
5. Double-click the software executable program again, and enable the instrument with device number 1 in the new window.

Note: If only one instrument is connected for use later, reset "DeviceNum" in the "configuration/Setting.ini" file to 0, otherwise the software may not recognize the instrument correctly.

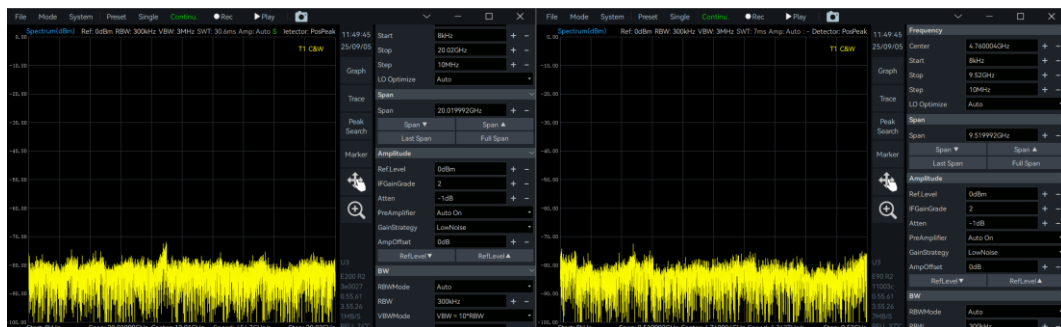


Figure 55 Operating two Instruments Simultaneously

# 16. Application for Options

## 16.1 Pulse Detection Option

### 16.1.1 Application for License

1. Refer to the [Viewing Instrument Information](#) section to view the soft and firmware version;
2. Ensure the version meets the following requirements:
  - GUI Version: 4.3.55.6 or above
  - API Version: 0.55.55 or above
  - FPGA Version: 0.55.15 or above
  - MCU Version: 0.55.32 or above
3. If the soft and firmware version does not meet the above requirements, please refer to the section on [Software and Firmware Update](#) to update.
4. Click "System" -> "About", take a screenshot of the entire software interface, and send it to the official technical support team to apply for the corresponding device license.

### 16.1.2 License Placement

#### 1 . Place the Pulse detection license for SA/NX Series instruments

- 1) Copy the obtained Pulse Detection license to the "/bin/CalFile" folder of the software;
- 2) Restart the software. In the menu bar, click "Mode" -> "Power Detection", then enable "Pulse Det" in the main settings area to use the pulse signal detection function.

#### 2 . Place the Pulse detection license for PX Series instruments

- 1) Extract the obtained "Option" folder and copy it to a USB flash drive;
- 2) Click "File" -> "Exit" to quit the software operation interface;
- 3) Insert the USB flash drive into the instrument's USB port. When the "Removable medium is inserted" prompt box pops up, click "OK";
- 4) Enter the "Option" folder, click the "Optional" icon. When the terminal prompts "The option has been successfully installed!!!", it indicates that the pulse license has been successfully placed;

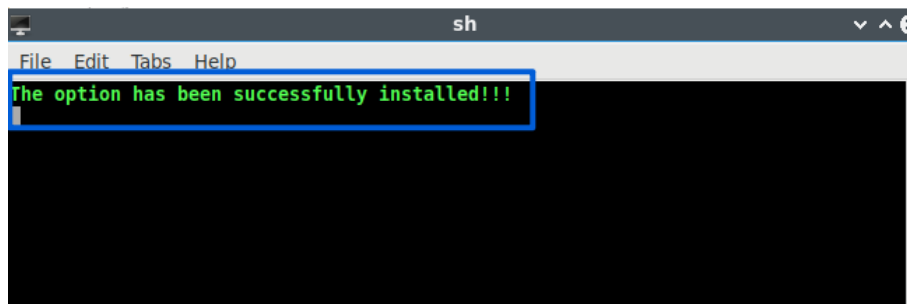


Figure 56 Install the Pulse Detection Option License

- 5) Close the popup window and restart the software. In the menu bar, click "Mode" -> "Pulse Detection", then enable "Pulse Det" in the main settings area to use the pulse signal detection function.

## 16.2 Digital Demodulation Option

### 16.2.1 Application for License and Digital Demodulation Library

Refer to the [license application for Pulse Signal Detection](#) to apply for the corresponding license and digital demodulation library.

### 16.2.2 License and Digital Demodulation Library Placement

#### 1 . Place the Digital demodulation license and Library for SA/NX Series instruments

- 1) Copy the "DigitalSigDemod.dll" demodulation library file into the "/bin" folder under the software directory;
- 2) Copy the digital demodulation license into the "/bin/CalFile" folder under the software directory;
- 3) Restart the software. In the menu bar, click "Mode" -> "Digital Demod" to enable and use the digital demodulation function.

#### 2 . Place the Digital demodulation license and Library for PX Series instruments

- 1) Refer to the [Place the Pulse detection license for PX Series Instruments](#) section, and click "Optional" icon to install the corresponding license and demodulation library;
- 2) Close the popup window and start the software. In the menu bar, click "Mode" -> "Digital Demod" to use the digital demodulation function.

## 16.3 AUXS Option

For later purchases of the ASG option, the device must be returned for an upgrade.

## 16.4 EMI Pre-Compliance Measurement Option

### 16.4.1 Apply for a License

1. Refer to the chapter on [Viewing Instrument Information](#) to check the software version;
2. Ensure that the GUI version is 4.4.55.52 or later;
3. If the software version does not meet the above requirement, refer to the chapter on [Software and Firmware Update](#) to upgrade it to the required version;
4. Click "System" -> "About", and send a screenshot of the entire software interface to official technical support to apply for the license for the corresponding device.

### 16.4.2 Place the License

#### 1 . Place the license for SA/NX Series instruments

- 1) Copy the EMI license obtained from Technical Support to the "/bin/CalFile" directory of the software installation folder;
- 2) Restart the software. In the menu bar, click "Mode" -> "EMI Pre-Compliance" to use the function.

#### 2 . Place the license for PX Series instruments

- 1) Refer to the [Place the Pulse detection license for PX Series Instruments](#) section, and click "Optional" icon to install the corresponding license and demodulation library;
- 2) Close the popup window and start the software. In the menu bar, click "Mode" -> "EMI Pre-Compliance" to use function.

## 17. Software and Firmware Update

This section describes how to update the instrument's software, FPGA, MCU, and Bus versions.

### 17.1 Version Requirements

1. Refer to the [viewing instrument information](#) section to check the software and firmware versions;
2. For all instruments, ensure that the GUI version is 4.4.55.39 or above;
3. If the software indicates that the update cannot be performed, please contact official technical support.

### 17.2 Parameter Description

**Note:** Displays the current and target versions of the software, FPGA, MCU, and Bus;

**Update Content:** Provides detailed information about the changes in the target version;

**Update Notification:** Sets whether to automatically pop up an update notification window when a new version is detected;

**Update Method:** The update methods are described in the table below.

**Table 30 Update Method Description**

| Update Method          | Description                                                                                                    |
|------------------------|----------------------------------------------------------------------------------------------------------------|
| Online Download        | Automatically connects to the remote server to download and install the latest software and firmware versions. |
| Use Built-in Firmware  | Restores the firmware version to the matching version corresponding to the current software.                   |
| Import Offline Package | Manually loads the update package from a USB flash drive or local storage media for installation.              |

### 17.3 Online Download

1. Click "System" -> "Update" to enter the update interface;
2. Check the "Update Notification" checkbox and ensure the device is connected to the internet. When the software starts or is running, if a new version is detected, the "Update" window will pop up automatically.
3. Set the "Update Method" to Online Download. The system will then start downloading the update package. You can monitor the progress on the download progress bar; during this process, the "Update" button will be temporarily disabled. After the package is successfully downloaded and parsed, detailed release notes will be displayed in the window, and the "Update" button will become enabled;
4. Carefully compare the information between the current version and the target version, and review the new features and fix list. Once confirmed, click the "Update" button in the lower-right corner;

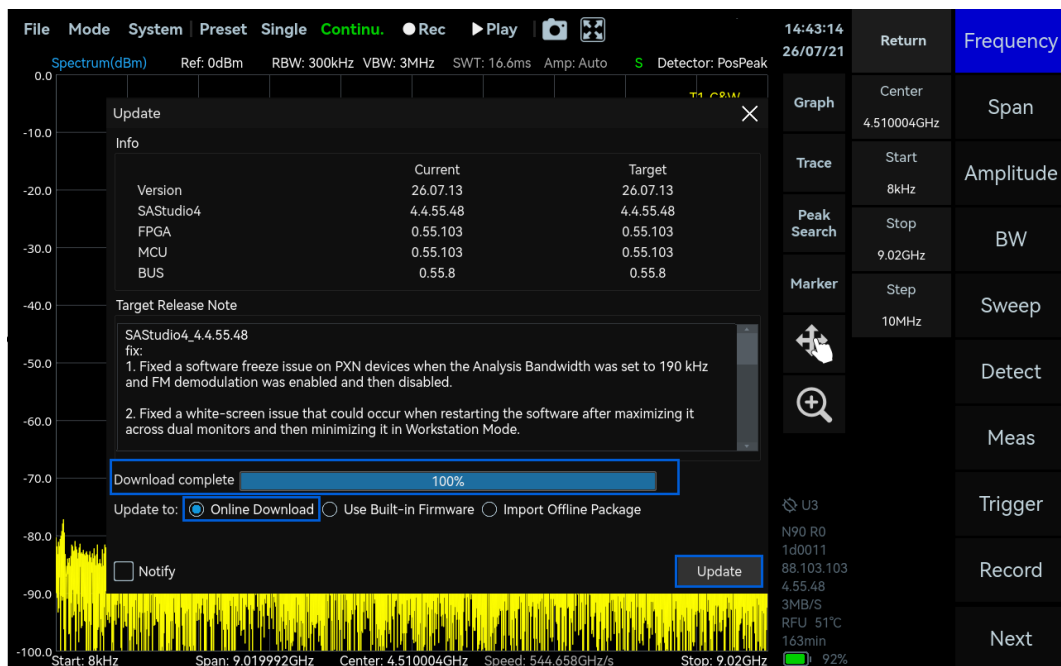


Figure 57 Update Software and Firmware Online

5. After clicking the "Update", the software will automatically exit and enter the upgrade process. Please keep the update window open until the progress bar completes and the software automatically restarts and returns to the main interface;
6. Close the update information window, then click "System" -> "About" in the menu bar to view the current firmware version of the instrument.

#### 17.4 Import Offline Package

Download the latest software version from the company's official website using the links below:

- <https://www.harogic.com/software-for-harogic-sa-nx-series-spectrum-analyzer/>

Taking the PX series instrument software and firmware update as an example, the offline update steps are as follows:

1. Copy the downloaded PX series software installation package from the official website to a USB drive. Insert the USB drive into the instrument, and click "OK" in the pop-up "Removable medium is inserted" window;
2. Click "System" -> "Update" to open the update window;
3. Select "Import Offline Package", click "Open" to choose the target software installation package, then click the "update" button at the bottom right;

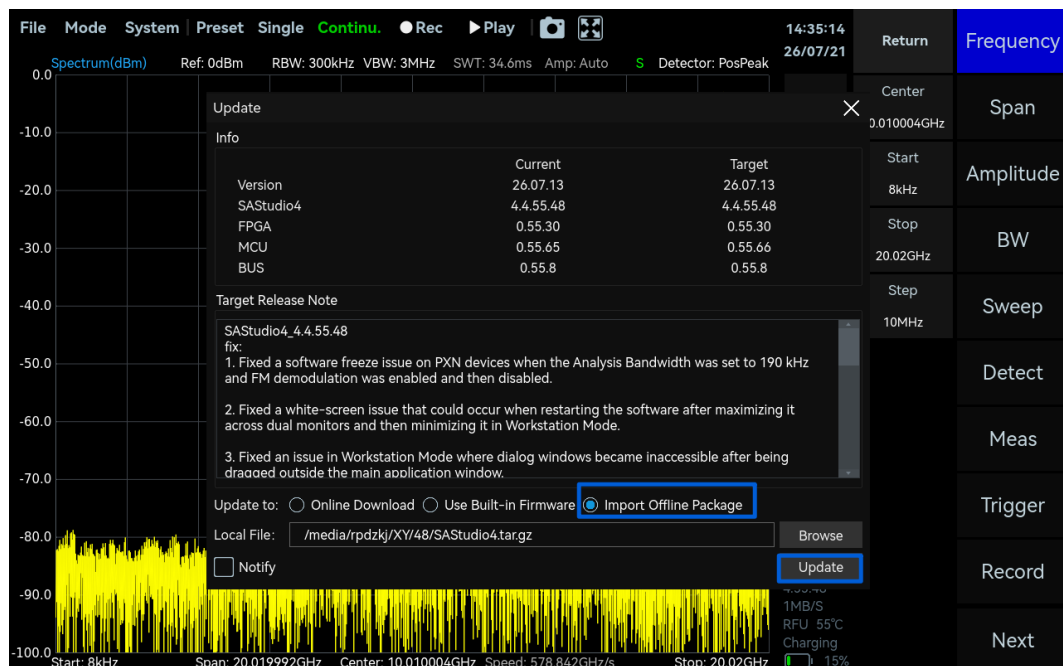


Figure 58 Offline Software and Firmware Update

4. The software will then automatically exit and enter the upgrade process. Please keep the update window open until the progress bar is complete and the software automatically restarts and returns to the main interface.

# Appendix

## Appendix 1: Record File Format Description

### 1.1 File Naming Format

The file name consists of the last four digits of the device ID, the date and time (year, month, day, hour, minute, and second) at the start of recording, the part index, and the file suffix.

For example: 0028\_yyyymmdd\_hhmmss\_partx. suffix.

Regardless of the total recording duration, all sub-files generated during the same recording session share the same date-time stamp in their names, which corresponds to the time when the recording started.

### 1.2 Conversion of Structures into Byte Arrays

The structures `SWP_Profile_TypeDef`, `SWP_TraceInfo_TypeDef`, `IQS_Profile_TypeDef`, `IQS_StreamInfo_TypeDef`, `DET_Profile_TypeDef`, `DET_StreamInfo_TypeDef`, `RTA_Profile_TypeDef` and `RTA_FrameInfo_TypeDef` are converted into byte arrays using the third-party tool msgpack. Therefore, these structures must also be decoded using msgpack during data reading.

## Appendix 2: Standard Spectrum Analysis Mode

The SWP record file uses a custom ".spectrum" format. The format description is shown in the following table.

**Table 1 Description of the Spectrum Format**

| Byte Index                                     | Description                                                                                                                                                                                                                      |
|------------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 0 to (71 + 10M)                                | This section stores the file information and packet index. (1 MB = 1024 * 1024 bytes)                                                                                                                                            |
| (72 + 10M) to (73+10M+length)                  | This section stores the SWP_Profile_TypeDef, SWP_Profile_TypeDef (default configuration), and SWP_TraceInfo_TypeDef structures, where length represents the total number of bytes occupied by these three structures.            |
| (74 + 10M + structure length) to (end of file) | This section stores the byte length of each data packet and the SWP data packets sequentially. Each SWP data packet mainly contains the frequency and power arrays, HopIndex, FrameIndex, and the MeasAuxInfo_TypeDef structure. |

**Table 2 Detailed Description of the Spectrum Format**

|                                              | Byte Index | Byte Count         | Data Type | Field Name                                                                                        | Endianness |
|----------------------------------------------|------------|--------------------|-----------|---------------------------------------------------------------------------------------------------|------------|
| File Header Information                      | 0          | 2                  | uint16_t  | File ID                                                                                           | Big Endian |
|                                              | 2          | 1                  | uint8_t   | 0x8c                                                                                              | Big Endian |
|                                              | 3          | 1                  | uint8_t   | 0x22                                                                                              | Big Endian |
|                                              | 4          | 1                  | uint8_t   | 0x52                                                                                              | Big Endian |
|                                              | 5          | 1                  | uint8_t   | 0x9b                                                                                              | Big Endian |
|                                              | 6          | 1                  | uint8_t   | 0x00 Protocol Version                                                                             | Big Endian |
|                                              | 7          | 1                  | uint8_t   | 0x01 Protocol Version                                                                             | Big Endian |
|                                              | 8          | 4                  | uint32_t  | api Version Information                                                                           | Big Endian |
|                                              | 9-63       | 56                 |           | Reserved                                                                                          |            |
|                                              | 64         | 8                  | quint64   | Number of Data Packets in Current File                                                            | Big Endian |
|                                              | 72         | 10M = 10*1024*1024 | QList     | Packet Index                                                                                      | Big Endian |
| Configuration Information msgpack Byte Array | 72+10M     | 2                  | uint16_t  | Configuration Information + Default Configuration Information + Trace Information Length (length) | Big Endian |
|                                              | 74+10M     |                    | double    | StartFreq_Hz                                                                                      |            |
|                                              |            |                    | double    | StopFreq_Hz                                                                                       |            |
|                                              |            |                    | double    | CenterFreq_Hz                                                                                     |            |
|                                              |            |                    | double    | Span_Hz                                                                                           |            |
|                                              |            |                    | double    | RefLevel_dBm                                                                                      |            |

|  | Byte Index | Byte Count | Data Type | Field Name                   | Endianness |
|--|------------|------------|-----------|------------------------------|------------|
|  |            |            | double    | RBW_Hz                       |            |
|  |            |            | double    | VBW_Hz                       |            |
|  |            |            | double    | SweepTime                    |            |
|  |            |            | double    | TraceBinSize_Hz              |            |
|  |            |            | int       | FreqAssignment               |            |
|  |            |            | int       | Window                       |            |
|  |            |            | int       | RBWMode                      |            |
|  |            |            | int       | VBWMode                      |            |
|  |            |            | int       | SweepTimeMode                |            |
|  |            |            | int       | Detector                     |            |
|  |            |            | int       | TraceFormat                  |            |
|  |            |            | int       | TraceDetectMode              |            |
|  |            |            | int       | TraceDetector                |            |
|  |            |            | uint32_t  | TracePoints                  |            |
|  |            |            | int       | TracePointsStrategy          |            |
|  |            |            | int       | TraceAlign                   |            |
|  |            |            | int       | FFTExecutionStrategy         |            |
|  |            |            | int       | RxPort                       |            |
|  |            |            | int       | SpurRejection                |            |
|  |            |            | int       | ReferenceClockSource         |            |
|  |            |            | double    | ReferenceClockFrequency      |            |
|  |            |            | uint8_t   | EnableReferenceClockOut      |            |
|  |            |            | int       | SystemClockSource            |            |
|  |            |            | double    | ExternalSystemClockFrequency |            |
|  |            |            | int       | TriggerSource                |            |
|  |            |            | int       | TriggerEdge                  |            |
|  |            |            | int       | TriggerOutMode               |            |
|  |            |            | int       | TriggerOutPulsePolarity      |            |
|  |            |            | uint32_t  | PowerBalance                 |            |
|  |            |            | int       | GainStrategy                 |            |
|  |            |            | int       | Preamplifier                 |            |

|                                                            | Byte Index                                                   | Byte Count | Data Type | Field Name                                        | Endianness         |
|------------------------------------------------------------|--------------------------------------------------------------|------------|-----------|---------------------------------------------------|--------------------|
|                                                            |                                                              |            | uint8_t   | AnalogIFBWGrade                                   |                    |
|                                                            |                                                              |            | uint8_t   | IFGainGrade                                       |                    |
|                                                            |                                                              |            | uint8_t   | EnableDebugMode                                   |                    |
|                                                            |                                                              |            | uint8_t   | CalibrationSettings                               |                    |
|                                                            |                                                              |            | int8_t    | Atten                                             |                    |
|                                                            |                                                              |            | int       | TraceType                                         |                    |
|                                                            |                                                              |            | int       | LOOptimization                                    |                    |
| Default Configuration Information<br>msgpack<br>Byte Array | Parameters Same as <a href="#">Configuration Information</a> |            |           |                                                   |                    |
| Trace Information<br>msgpack<br>Byte Array                 |                                                              |            | int       | FullsweepTracePoints                              |                    |
|                                                            |                                                              |            | int       | PartialsweepTracePoints                           |                    |
|                                                            |                                                              |            | int       | TotalHops                                         |                    |
|                                                            |                                                              |            | uint32_t  | UserStartIndex                                    |                    |
|                                                            |                                                              |            | uint32_t  | UserStopIndex                                     |                    |
|                                                            |                                                              |            | double    | TraceBinBW_Hz                                     |                    |
|                                                            |                                                              |            | double    | StartFreq_Hz                                      |                    |
|                                                            |                                                              |            | double    | AnalysisBW_Hz                                     |                    |
|                                                            |                                                              |            | int       | TraceDetectRatio                                  |                    |
|                                                            |                                                              |            | int       | DecimateFactor                                    |                    |
|                                                            |                                                              |            | float     | FrameTimeMultiple                                 |                    |
|                                                            |                                                              |            | double    | FrameTime                                         |                    |
|                                                            |                                                              |            | double    | EstimateMinSweepTime                              |                    |
|                                                            |                                                              |            | int       | DataFormat                                        |                    |
|                                                            |                                                              |            | uint64_t  | SamplePoints                                      |                    |
|                                                            |                                                              |            | uint32_t  | GainParameter                                     |                    |
|                                                            |                                                              |            | int       | DSPPlatform                                       |                    |
| Data Packet                                                | 74+10M+ <a href="#">length</a>                               | 4          | int       | Data Packet Length                                | Big Endian         |
|                                                            |                                                              | 8*N        | double*N  | Frequency Array<br>(N = PartialsweepTrace Points) | Platform Dependent |
|                                                            |                                                              | 4*N        | float*N   | Power Array<br>(N = PartialsweepTrace Points)     | Platform Dependent |
|                                                            |                                                              | 4          | int       | HopIndex                                          | Big Endian         |

|                                                                                        | Byte Index | Byte Count | Data Type | Field Name         | Endianness |
|----------------------------------------------------------------------------------------|------------|------------|-----------|--------------------|------------|
|                                                                                        |            | 4          | int       | FrameIndex         | Big Endian |
|                                                                                        |            | 4          | uint32_t  | MaxIndex           | Big Endian |
|                                                                                        |            | 4          | float     | MaxPower_dBm       | Big Endian |
|                                                                                        |            | 2          | int16_t   | Temperature        | Big Endian |
|                                                                                        |            | 2          | uint16_t  | RFState            | Big Endian |
|                                                                                        |            | 2          | uint16_t  | BBState            | Big Endian |
|                                                                                        |            | 2          | uint16_t  | GainPattern        | Big Endian |
|                                                                                        |            | 4          | uint32_t  | ConvertPattern     | Big Endian |
|                                                                                        |            | 8          | double    | SysTimeStamp       | Big Endian |
|                                                                                        |            | 8          | double    | AbsoluteTimeStamp  | Big Endian |
|                                                                                        |            | 4          | float     | Latitude           | Big Endian |
|                                                                                        |            | 4          | float     | Longitude          | Big Endian |
|                                                                                        |            |            |           |                    |            |
| <b>Next Data Packet</b><br>The total number of packets can be found in the File Header |            | 4          | int       | Data Packet Length | Big Endian |
|                                                                                        |            |            |           | ...                |            |

## Appendix 3: Receiver/IQ Stream Mode

The IQ record file uses the standard ".wav" format. The format description is shown in the following table.

**Table 3 Description of the WAV Format**

| Chunk                           | Description                                                                                                                                                                                                                        |
|---------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>RIFF chunk</b>               |                                                                                                                                                                                                                                    |
| <b>RIFF chunk size</b>          |                                                                                                                                                                                                                                    |
| <b>File Format Type: "WAVE"</b> |                                                                                                                                                                                                                                    |
| <b>fmt chunk</b>                |                                                                                                                                                                                                                                    |
| <b>fmt chunk size</b>           |                                                                                                                                                                                                                                    |
| <b>fmt chunk data</b>           |                                                                                                                                                                                                                                    |
| <b>prof chunk</b>               | Format Chunk Identifier: "prof"                                                                                                                                                                                                    |
| <b>prof chunk size</b>          | Chunk Length                                                                                                                                                                                                                       |
| <b>prof chunk data</b>          | This chunk stores the IQS_Profile_TypeDef, IQS_StreamInfo_TypeDef, DeviceInfo_TypeDef, and other related information.                                                                                                              |
| <b>trig chunk</b>               | Format Chunk Identifier: "trig"                                                                                                                                                                                                    |
| <b>trig chunk size</b>          | Chunk Length                                                                                                                                                                                                                       |
| <b>trig chunk data</b>          | This chunk stores the IQS_TriggerInfo_TypeDef, DeviceState_TypeDef, IQS_ScaleToV, MaxPower_dBm, and MaxIndex for each IQ data packet, sequentially arranged. Each entry corresponds one-to-one with the packets in the data chunk. |
| <b>data chunk</b>               | Format Chunk Identifier: "data"                                                                                                                                                                                                    |
| <b>data chunk size</b>          | Chunk Length                                                                                                                                                                                                                       |
| <b>data chunk data</b>          | This chunk stores the IQ data packets in sequential order.                                                                                                                                                                         |

**Table 4 Detailed Description of the iq.wav Format**

|                                            | Chunk | Byte Index | Byte Index within Chunk | Byte Count | Data Type | Field Name                                         | Field Description | Endianness    |
|--------------------------------------------|-------|------------|-------------------------|------------|-----------|----------------------------------------------------|-------------------|---------------|
| RIFF File Header Information               | RIFF  | 0          |                         | 4          |           | Document Identifier                                | "RIFF"            |               |
|                                            |       | 4          |                         | 4          | uint32_t  | Data Length                                        | Chunk Length      | Litter Endian |
|                                            |       | 8          |                         | 4          |           | File Format Type                                   | "WAVE"            |               |
| fmt Chunk Description                      | fmt   | 12         |                         | 4          |           | Format Chunk Identifier                            | "fmt"             |               |
|                                            |       | 16         |                         | 4          | uint32_t  | Chunk Length                                       | 16                | Litter Endian |
|                                            |       | 20         |                         | 2          | uint16_t  | Audio Format Code                                  | 1                 | Litter Endian |
|                                            |       | 22         |                         | 2          | uint16_t  |                                                    | 2                 | Litter Endian |
|                                            |       | 24         |                         | 4          | uint32_t  | Sampling Frequency                                 |                   | Litter Endian |
|                                            |       | 28         |                         | 4          | uint32_t  | Byte Rate                                          |                   | Litter Endian |
|                                            |       | 32         |                         | 2          | uint16_t  | Block Align                                        |                   | Litter Endian |
|                                            |       | 34         |                         | 2          | uint16_t  | Bits per Sample                                    |                   | Litter Endian |
| File Header Information                    | prof  | 36         |                         | 4          |           | Format Chunk Identifier                            | "prof"            |               |
|                                            |       | 40         |                         | 4          | uint32_t  | Chunk Length                                       |                   | Litter Endian |
|                                            |       | 44         | 0                       | 2          | uint16_t  | File ID                                            |                   | Big Endian    |
|                                            |       | 46         | 2                       | 1          | uint8_t   | 0x8c                                               |                   | Big Endian    |
|                                            |       | 47         | 3                       | 1          | uint8_t   | 0x22                                               |                   | Big Endian    |
|                                            |       | 48         | 4                       | 1          | uint8_t   | 0x52                                               |                   | Big Endian    |
|                                            |       | 49         | 5                       | 1          | uint8_t   | 0x9b                                               |                   | Big Endian    |
|                                            |       | 50         | 6                       | 1          | uint8_t   | 0x00 Protocol Version                              |                   | Big Endian    |
|                                            |       | 51         | 7                       | 1          | uint8_t   | 0x02 Protocol Version                              |                   | Big Endian    |
|                                            |       | 52         | 8                       | 4          | uint32_t  | api Version Information                            |                   | Big Endian    |
|                                            |       | 53-107     | 56                      |            |           | Reserved                                           |                   |               |
| IQS_Profile Information msgpack Byte Array |       | 108        | 64                      | 2          | uint16_t  | IQS_Profile + IQS_StreamInfo Structure Byte Length |                   | Big Endian    |
|                                            |       | 110        | 66                      |            | double    | CenterFreq_Hz                                      |                   |               |
|                                            |       |            |                         |            | double    | RefLevel_dBm                                       |                   |               |
|                                            |       |            |                         |            | uint32_t  | DecimateFactor                                     |                   |               |
|                                            |       |            |                         |            | int       | RxPort                                             |                   |               |
|                                            |       |            |                         |            | uint32_t  | BusTimeout_ms                                      |                   |               |

|  | Chunk | Byte Index | Byte Index within Chunk | Byte Count | Data Type | Field Name                   | Field Description | Endianness |
|--|-------|------------|-------------------------|------------|-----------|------------------------------|-------------------|------------|
|  |       |            |                         |            | int       | TriggerSource                |                   |            |
|  |       |            |                         |            | int       | TriggerEdge                  |                   |            |
|  |       |            |                         |            | int       | TriggerMode                  |                   |            |
|  |       |            |                         |            | uint64_t  | TriggerLength                |                   |            |
|  |       |            |                         |            | int       | TriggerOutMode               |                   |            |
|  |       |            |                         |            | int       | TriggerOutPulsePolarity      |                   |            |
|  |       |            |                         |            | double    | TriggerLevel_dBm             |                   |            |
|  |       |            |                         |            | double    | TriggerLevel_SafeTime        |                   |            |
|  |       |            |                         |            | double    | TriggerDelay                 |                   |            |
|  |       |            |                         |            | double    | PreTriggerTime               |                   |            |
|  |       |            |                         |            | int       | TriggerTimerSync             |                   |            |
|  |       |            |                         |            | double    | TriggerTimer_Period          |                   |            |
|  |       |            |                         |            | uint8_t   | EnableReTrigger              |                   |            |
|  |       |            |                         |            | double    | ReTrigger_Period             |                   |            |
|  |       |            |                         |            | uint16_t  | ReTrigger_Count              |                   |            |
|  |       |            |                         |            | int       | DataFormat                   |                   |            |
|  |       |            |                         |            | int       | GainStrategy                 |                   |            |
|  |       |            |                         |            | int       | Preamplifier                 |                   |            |
|  |       |            |                         |            | uint8_t   | AnalogIFBWGrade              |                   |            |
|  |       |            |                         |            | uint8_t   | IFGainGrade                  |                   |            |
|  |       |            |                         |            | uint8_t   | EnableDebugMode              |                   |            |
|  |       |            |                         |            | int       | ReferenceClockSource         |                   |            |
|  |       |            |                         |            | double    | ReferenceClockFrequency      |                   |            |
|  |       |            |                         |            | uint8_t   | EnableReferenceClockOut      |                   |            |
|  |       |            |                         |            | int       | SystemClockSource            |                   |            |
|  |       |            |                         |            | double    | ExternalSystemClockFrequency |                   |            |
|  |       |            |                         |            | double    | NativeQSampleRate_SPS        |                   |            |
|  |       |            |                         |            | uint8_t   | EnableIFAGC                  |                   |            |
|  |       |            |                         |            | int8_t    | Atten                        |                   |            |
|  |       |            |                         |            | int       | DCCancelerMode               |                   |            |

|                                                                         | Chunk | Byte Index | Byte Index within Chunk | Byte Count | Data Type | Field Name                            | Field Description | Endianness         |
|-------------------------------------------------------------------------|-------|------------|-------------------------|------------|-----------|---------------------------------------|-------------------|--------------------|
|                                                                         |       |            |                         |            | int       | QDCMode                               |                   |                    |
|                                                                         |       |            |                         |            | float     | QDCIGain                              |                   |                    |
|                                                                         |       |            |                         |            | float     | QDCQGain                              |                   |                    |
|                                                                         |       |            |                         |            | float     | QDCPhaseComp                          |                   |                    |
|                                                                         |       |            |                         |            | int8_t    | DCCIOffset                            |                   |                    |
|                                                                         |       |            |                         |            | int8_t    | DCCQOffset                            |                   |                    |
|                                                                         |       |            |                         |            | int       | LOOptimization                        |                   |                    |
| IQS_<br>StreamInfo<br>Structure<br>Information<br>msgpack<br>Byte Array |       |            |                         |            | double    | Bandwidth                             |                   |                    |
|                                                                         |       |            |                         |            | double    | IQSampleRate                          |                   |                    |
|                                                                         |       |            |                         |            | uint64_t  | PacketCount                           |                   |                    |
|                                                                         |       |            |                         |            | uint64_t  | StreamSamples                         |                   |                    |
|                                                                         |       |            |                         |            | uint64_t  | StreamDataSize                        |                   |                    |
|                                                                         |       |            |                         |            | uint32_t  | PacketSamples                         |                   |                    |
|                                                                         |       |            |                         |            | uint32_t  | PacketDataSize                        |                   |                    |
|                                                                         |       |            |                         |            | uint32_t  | GainParameter                         |                   |                    |
| DeviceInfo<br>Structure<br>Information                                  |       |            |                         | 2          | uint16_t  | DeviceInfo Structure Byte Length      |                   | Big Endian         |
|                                                                         |       |            |                         | 8          | uint64_t  | DeviceUID                             |                   | Big Endian         |
|                                                                         |       |            |                         | 2          | uint16_t  | Model                                 |                   | Big Endian         |
|                                                                         |       |            |                         | 2          | uint16_t  | HardwareVersion                       |                   | Big Endian         |
|                                                                         |       |            |                         | 4          | uint32_t  | MFWVersion                            |                   | Big Endian         |
|                                                                         |       |            |                         | 4          | uint32_t  | FFWVersion                            |                   | Big Endian         |
| Reserved                                                                |       |            |                         |            |           |                                       |                   |                    |
| IQS_<br>TriggerInfo<br>Structure<br>Information                         | trig  | 400        |                         | 4          |           | Chunk Identifier                      | "trig"            |                    |
|                                                                         |       | 404        |                         | 4          | uint32_t  | Chunk Length                          |                   | Little Endian      |
|                                                                         |       | 408        |                         | 2          | uint16_t  | IQS_TriggerInfo Structure Byte Length |                   | Big Endian         |
|                                                                         |       |            |                         | 8          | uint64_t  | SysTimerCountOfFirstDataPoint         |                   | Big Endian         |
|                                                                         |       |            |                         | 2          | uint16_t  | InPacketTriggeredDataSize             |                   | Big Endian         |
|                                                                         |       |            |                         | 2          | uint16_t  | InPacketTriggerEdges                  |                   | Big Endian         |
|                                                                         |       |            |                         | 4*25       | uint32_t  | StartDataIndexOfTriggerEdges[25]      |                   | Platform Dependent |
|                                                                         |       |            |                         | 8*25       | uint64_t  | SysTimerCountOfEdges[25]              |                   | Platform Dependent |

|                                   | Chunk | Byte Index       | Byte Index within Chunk | Byte Count | Data Type | Field Name                                               | Field Description | Endianness         |
|-----------------------------------|-------|------------------|-------------------------|------------|-----------|----------------------------------------------------------|-------------------|--------------------|
| DeviceState Structure Information |       |                  |                         | 25         | int8_t    | EdgeType[25]                                             |                   | Platform Dependent |
|                                   |       |                  |                         | 2          | uint16_t  | DeviceState Structure Byte Length                        |                   | Big Endian         |
|                                   |       |                  |                         | 2          | int16_t   | Temperature                                              |                   | Big Endian         |
|                                   |       |                  |                         | 2          | uint16_t  | RFState                                                  |                   | Big Endian         |
|                                   |       |                  |                         | 2          | uint16_t  | BBState                                                  |                   | Big Endian         |
|                                   |       |                  |                         | 8          | double    | AbsoluteTimeStamp                                        |                   | Big Endian         |
|                                   |       |                  |                         | 4          | float     | Latitude                                                 |                   | Big Endian         |
|                                   |       |                  |                         | 4          | float     | Longitude                                                |                   | Big Endian         |
|                                   |       |                  |                         | 2          | uint16_t  | GainPattern                                              |                   | Big Endian         |
|                                   |       |                  |                         | 8          | int64_t   | RFCFreq                                                  |                   | Big Endian         |
|                                   |       |                  |                         | 4          | uint32_t  | ConvertPattern                                           |                   | Big Endian         |
|                                   |       |                  |                         | 4          | uint32_t  | NCOFTW                                                   |                   | Big Endian         |
|                                   |       |                  |                         | 4          | uint32_t  | SampleRate                                               |                   | Big Endian         |
|                                   |       |                  |                         | 2          | uint16_t  | CPU_BCFlag                                               |                   | Big Endian         |
|                                   |       |                  |                         | 2          | uint16_t  | IFOverflow                                               |                   | Big Endian         |
|                                   |       |                  |                         | 2          | uint16_t  | DecimateFactor                                           |                   | Big Endian         |
|                                   |       |                  |                         | 2          | uint16_t  | OptionState                                              |                   | Big Endian         |
| Return Information                |       |                  |                         | 4          | float     | IQS_ScaleToV                                             |                   | Big Endian         |
|                                   |       |                  |                         | 4          | float     | MaxPower_dBm                                             |                   | Big Endian         |
|                                   |       |                  |                         | 4          | uint32_t  | MaxIndex                                                 |                   | Big Endian         |
| Reserved                          |       |                  |                         |            |           |                                                          |                   |                    |
| Data Packet                       | Data  | 25*1024*1024+400 |                         | 4          |           | Chunk Identifier                                         | "data"            |                    |
|                                   |       | 25*1024*1024+404 |                         | 4          | uint32_t  | Chunk Length                                             |                   | Little Endian      |
|                                   |       | 25*1024*1024+408 |                         | 64968      |           | IQ Data Packet                                           |                   | Platform Dependent |
|                                   |       |                  |                         | 64968      |           | IQ Data Packet                                           |                   | Platform Dependent |
|                                   |       |                  |                         |            |           | ...                                                      |                   | Platform Dependent |
|                                   |       |                  |                         |            |           | The Nth IQ Data Packet, where N = (Chunk Length / 64968) |                   | Platform Dependent |

## Appendix 4: Power Detection Mode

The DET record file uses the standard ".wav" format, but it is not playable by third-party software. The format description is shown in the following table.

**Table 5 Description of the WAV Format**

| Chunk                           | Description                                                                                                                                                                                                                        |
|---------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>RIFF chunk</b>               |                                                                                                                                                                                                                                    |
| <b>RIFF chunk size</b>          |                                                                                                                                                                                                                                    |
| <b>File Format Type: "WAVE"</b> |                                                                                                                                                                                                                                    |
| <b>fmt chunk</b>                |                                                                                                                                                                                                                                    |
| <b>fmt chunk size</b>           |                                                                                                                                                                                                                                    |
| <b>fmt chunk data</b>           |                                                                                                                                                                                                                                    |
| <b>prof chunk</b>               | Format Chunk Identifier: "prof"                                                                                                                                                                                                    |
| <b>prof chunk size</b>          | Chunk Length                                                                                                                                                                                                                       |
| <b>prof chunk data</b>          | This chunk stores the IQS_Profile_TypeDef, IQS_StreamInfo_TypeDef, DeviceInfo_TypeDef, and other related information.                                                                                                              |
| <b>trig chunk</b>               | Format Chunk Identifier: "trig"                                                                                                                                                                                                    |
| <b>trig chunk size</b>          | Chunk Length                                                                                                                                                                                                                       |
| <b>trig chunk data</b>          | This chunk stores the IQS_TriggerInfo_TypeDef, DeviceState_TypeDef, IQS_ScaleToV, MaxPower_dBm, and MaxIndex for each IQ data packet, arranged sequentially. Each entry corresponds one-to-one with the packets in the data chunk. |
| <b>data chunk</b>               | Format Chunk Identifier: "data"                                                                                                                                                                                                    |
| <b>data chunk size</b>          | Chunk Length                                                                                                                                                                                                                       |
| <b>data chunk data</b>          | This chunk stores the IQ data packets in sequential order.                                                                                                                                                                         |

**Table 6 Detailed Description of the iq.wav Format**

|                                                            | Chunk | Byte Index | Byte Index within Chunk | Byte Count | Data Type | Field Name                                         | Filed Description | Endianness    |
|------------------------------------------------------------|-------|------------|-------------------------|------------|-----------|----------------------------------------------------|-------------------|---------------|
| RIFF File Header Information                               | RIFF  | 0          |                         | 4          |           | Document Identifier                                | "RIFF"            |               |
|                                                            |       | 4          |                         | 4          | uint32_t  | Data Length                                        | Chunk Length      | Litter Endian |
|                                                            |       | 8          |                         | 4          |           | File Format Type                                   | "WAVE"            |               |
| fmt Format Chunk Structure Description                     | fmt   | 12         |                         | 4          |           | Format Chunk Identifier                            | "fmt "            |               |
|                                                            |       | 16         |                         | 4          | uint32_t  | Chunk Length                                       | 16                | Litter Endian |
|                                                            |       | 20         |                         | 2          | uint16_t  | Audio Format Code                                  | 1                 | Litter Endian |
|                                                            |       | 22         |                         | 2          | uint16_t  | Number of Channels                                 | 2                 | Litter Endian |
|                                                            |       | 24         |                         | 4          | uint32_t  | Sampling Frequency                                 |                   | Litter Endian |
|                                                            |       | 28         |                         | 4          | uint32_t  | Byte Rate                                          |                   | Litter Endian |
|                                                            |       | 32         |                         | 2          | uint16_t  | Block Align                                        |                   | Litter Endian |
|                                                            |       | 34         |                         | 2          | uint16_t  | Bits per Sample                                    |                   | Litter Endian |
| File Header Information                                    | prof  | 36         |                         | 4          |           | Format Chunk Identifier                            | "prof"            |               |
|                                                            |       | 40         |                         | 4          | uint32_t  | Chunk Length                                       |                   | Litter Endian |
|                                                            |       | 44         | 0                       | 2          | uint16_t  | File ID                                            |                   | Big Endian    |
|                                                            |       | 46         | 2                       | 1          | uint8_t   | 0x8c                                               |                   | Big Endian    |
|                                                            |       | 47         | 3                       | 1          | uint8_t   | 0x22                                               |                   | Big Endian    |
|                                                            |       | 48         | 4                       | 1          | uint8_t   | 0x52                                               |                   | Big Endian    |
|                                                            |       | 49         | 5                       | 1          | uint8_t   | 0x9b                                               |                   | Big Endian    |
|                                                            |       | 50         | 6                       | 1          | uint8_t   | 0x00 Protocol Version                              |                   | Big Endian    |
|                                                            |       | 51         | 7                       | 1          | uint8_t   | 0x04 Protocol Version                              |                   | Big Endian    |
|                                                            |       | 52         | 8                       | 4          | uint32_t  | api Version Information                            |                   | Big Endian    |
|                                                            |       | 53-107     | 56                      |            |           | Reserved                                           |                   |               |
| DET_Profile Structure Information<br>msgpack<br>Byte Array |       | 108        | 64                      | 2          | uint16_t  | DET_Profile + DET_StreamInfo Structure Byte Length |                   | Big Endian    |
|                                                            |       | 110        | 66                      |            | double    | CenterFreq_Hz                                      |                   |               |
|                                                            |       |            |                         |            | double    | RefLevel_dBm                                       |                   |               |
|                                                            |       |            |                         |            | uint32_t  | DecimateFactor                                     |                   |               |
|                                                            |       |            |                         |            | int       | RxPort                                             |                   |               |
|                                                            |       |            |                         |            | uint32_t  | BusTimeout_ms                                      |                   |               |
|                                                            |       |            |                         |            | int       | TriggerSource                                      |                   |               |

|  | Chunk | Byte Index | Byte Index within Chunk | Byte Count | Data Type | Field Name                   | Field Description | Endianness |
|--|-------|------------|-------------------------|------------|-----------|------------------------------|-------------------|------------|
|  |       |            |                         |            | int       | TriggerEdge                  |                   |            |
|  |       |            |                         |            | int       | TriggerMode                  |                   |            |
|  |       |            |                         |            | uint64_t  | TriggerLength                |                   |            |
|  |       |            |                         |            | int       | TriggerOutMode               |                   |            |
|  |       |            |                         |            | int       | TriggerOutPulsePolarity      |                   |            |
|  |       |            |                         |            | double    | TriggerLevel_dBm             |                   |            |
|  |       |            |                         |            | double    | TriggerLevel_SafeTime        |                   |            |
|  |       |            |                         |            | double    | TriggerDelay                 |                   |            |
|  |       |            |                         |            | double    | PreTriggerTime               |                   |            |
|  |       |            |                         |            | int       | TriggerTimerSync             |                   |            |
|  |       |            |                         |            | double    | TriggerTimer_Period          |                   |            |
|  |       |            |                         |            | uint8_t   | EnableReTrigger              |                   |            |
|  |       |            |                         |            | double    | ReTrigger_Period             |                   |            |
|  |       |            |                         |            | uint16_t  | ReTrigger_Count              |                   |            |
|  |       |            |                         |            | int       | Detector                     |                   |            |
|  |       |            |                         |            | uint16_t  | DetectRatio                  |                   |            |
|  |       |            |                         |            | int       | GainStrategy                 |                   |            |
|  |       |            |                         |            | int       | Preamplifier                 |                   |            |
|  |       |            |                         |            | uint8_t   | AnalogIFBWGrade              |                   |            |
|  |       |            |                         |            | uint8_t   | IFGainGrade                  |                   |            |
|  |       |            |                         |            | uint8_t   | EnableDebugMode              |                   |            |
|  |       |            |                         |            | int       | ReferenceClockSource         |                   |            |
|  |       |            |                         |            | double    | ReferenceClockFrequency      |                   |            |
|  |       |            |                         |            | uint8_t   | EnableReferenceClockOut      |                   |            |
|  |       |            |                         |            | int       | SystemClockSource            |                   |            |
|  |       |            |                         |            | double    | ExternalSystemClockFrequency |                   |            |
|  |       |            |                         |            | int8_t    | Atten                        |                   |            |
|  |       |            |                         |            | int       | DCCancelerMode               |                   |            |
|  |       |            |                         |            | int       | QDCMode                      |                   |            |
|  |       |            |                         |            | float     | QDCIGain                     |                   |            |

|                                                                                                     | Chunk | Byte Index | Byte Index with Chunk | Byte Count | Data Type | Field Name                            | Field Description | Endianness         |
|-----------------------------------------------------------------------------------------------------|-------|------------|-----------------------|------------|-----------|---------------------------------------|-------------------|--------------------|
|                                                                                                     |       |            |                       |            | float     | QDCQGain                              |                   |                    |
|                                                                                                     |       |            |                       |            | float     | QDCPhaseComp                          |                   |                    |
|                                                                                                     |       |            |                       |            | int8_t    | DCCIOffset                            |                   |                    |
|                                                                                                     |       |            |                       |            | int8_t    | DCCQOffset                            |                   |                    |
|                                                                                                     |       |            |                       |            | int       | LOOptimization                        |                   |                    |
| <b>DET_</b><br><b>StreamInfo</b><br><b>Structure</b><br><b>Information</b><br>msgpack<br>Byte Array |       |            |                       |            | uint64_t  | PacketCount                           |                   |                    |
|                                                                                                     |       |            |                       |            | uint64_t  | StreamSamples                         |                   |                    |
|                                                                                                     |       |            |                       |            | uint64_t  | StreamDataSize                        |                   |                    |
|                                                                                                     |       |            |                       |            | uint32_t  | PacketSamples                         |                   |                    |
|                                                                                                     |       |            |                       |            | uint32_t  | PacketDataSize                        |                   |                    |
|                                                                                                     |       |            |                       |            | double    | TimeResolution                        |                   |                    |
|                                                                                                     |       |            |                       |            | uint32_t  | GainParameter                         |                   |                    |
| <b>Reserved</b>                                                                                     |       |            |                       |            |           |                                       |                   |                    |
| <b>IQS_</b><br><b>TriggerInfo</b><br><b>Structure</b><br><b>Information</b>                         | trig  | 400        |                       | 4          |           | Format Chunk Identifier               | "trig"            |                    |
|                                                                                                     |       | 404        |                       | 4          | uint32_t  | Chunk Length                          |                   | Litter Endian      |
|                                                                                                     |       | 408        |                       | 2          | uint16_t  | IQS_TriggerInfo Structure Byte Length |                   | Big Endian         |
|                                                                                                     |       |            |                       | 8          | uint64_t  | SysTimerCountOfFirstDataPoint         |                   | Big Endian         |
|                                                                                                     |       |            |                       | 2          | uint16_t  | InPacketTriggeredDataSize             |                   | Big Endian         |
|                                                                                                     |       |            |                       | 2          | uint16_t  | InPacketTriggerEdges                  |                   | Big Endian         |
|                                                                                                     |       |            |                       | 4*25       | uint32_t  | StartDataIndexOfTriggerEdges[25]      |                   | Platform Dependent |
|                                                                                                     |       |            |                       | 8*25       | uint64_t  | SysTimerCountOfEdges[25]              |                   | Platform Dependent |
|                                                                                                     |       |            |                       | 25         | int8_t    | EdgeType[25]                          |                   | Platform Dependent |
| <b>MeasAuxInfo</b><br><b>Structure</b><br><b>Information</b>                                        |       |            |                       | 2          | uint16_t  | MeasAuxInfo Structure Byte Length     |                   | Big Endian         |
|                                                                                                     |       |            |                       | 4          | uint32_t  | MaxIndex                              |                   | Big Endian         |
|                                                                                                     |       |            |                       | 4          | float     | MaxPower_dBm                          |                   | Big Endian         |
|                                                                                                     |       |            |                       | 2          | int16_t   | Temperature                           |                   | Big Endian         |
|                                                                                                     |       |            |                       | 2          | uint16_t  | RFState                               |                   | Big Endian         |
|                                                                                                     |       |            |                       | 2          | uint16_t  | BBState                               |                   | Big Endian         |
|                                                                                                     |       |            |                       | 2          | uint16_t  | GainPattern                           |                   | Big Endian         |
|                                                                                                     |       |            |                       | 4          | uint32_t  | ConvertPattern                        |                   | Big Endian         |

|             | Chunk | Byte Index       | Byte Index within Chunk | Byte Count | Data Type | Field Name                                                | Field Description | Endianness         |
|-------------|-------|------------------|-------------------------|------------|-----------|-----------------------------------------------------------|-------------------|--------------------|
|             |       |                  |                         | 8          | double    | SysTimeStamp                                              |                   | Big Endian         |
|             |       |                  |                         | 8          | double    | AbsoluteTimeStamp                                         |                   | Big Endian         |
|             |       |                  |                         | 4          | float     | Latitude                                                  |                   | Big Endian         |
|             |       |                  |                         | 4          | float     | Longitude                                                 |                   | Big Endian         |
|             |       |                  |                         | 4          | float     | ScaleToV                                                  |                   | Big Endian         |
| Reserved    |       |                  |                         |            |           |                                                           |                   |                    |
| Data Packet | Data  | 25*1024*1024+400 |                         | 4          |           | Format Chunk Identifier                                   | "data"            |                    |
|             |       | 25*1024*1024+404 |                         | 4          | uint32_t  | Chunk Length                                              |                   | Little Endian      |
|             |       | 25*1024*1024+408 |                         | 64968      |           | DET Data Packet                                           |                   | Platform Dependent |
|             |       |                  |                         | 64968      |           | DET Data Packet                                           |                   | Platform Dependent |
|             |       |                  |                         |            |           | ...                                                       |                   | Platform Dependent |
|             |       |                  |                         |            |           | The Nth DET Data Packet, where N = (Chunk Length / 64968) |                   | Platform Dependent |

## Appendix 5: Real-Time Spectrum Analysis Mode

The RTA record file uses a custom ".rtspectrum" format. The format description is shown in the following table.

**Table 7 Description of the rtspectrum Format**

| Chunk                                    | Description                                                                                                                                                                                                                                      |
|------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>0 to (71+10M)</b>                     | This section stores the file information and packet index. (1 MB = 1024 × 1024 bytes)                                                                                                                                                            |
| <b>(72+10M) to (73+10M+ length)</b>      | This section stores the RTA_Profile_TypeDef and RTA_FrameInfo_TypeDef structures, where length represents the total number of bytes occupied by these structures.                                                                                |
| <b>(74+10M+ length) to (end of file)</b> | This section stores the byte length of each data packet and the RTA data packets sequentially. Each RTA data packet mainly contains the SpectrumStream array, RTA_PlotInfo_TypeDef, RTA_TriggerInfo_TypeDef, and MeasAuxInfo_TypeDef structures. |

**Table 8 Detailed Description of the rtspectrum Format**

|                                                    | Byte Index | Byte Count       | Data Type | Field Name                                                    | Endianness |
|----------------------------------------------------|------------|------------------|-----------|---------------------------------------------------------------|------------|
| File Header Information                            | 0          | 2                | uint16_t  | File ID                                                       | Big Endian |
|                                                    | 2          | 1                | uint8_t   | 0x8c                                                          | Big Endian |
|                                                    | 3          | 1                | uint8_t   | 0x22                                                          | Big Endian |
|                                                    | 4          | 1                | uint8_t   | 0x52                                                          | Big Endian |
|                                                    | 5          | 1                | uint8_t   | 0x9b                                                          | Big Endian |
|                                                    | 6          | 1                | uint8_t   | 0x00 Protocol Version                                         | Big Endian |
|                                                    | 7          | 1                | uint8_t   | 0x03 Protocol Version                                         | Big Endian |
|                                                    | 8          | 4                | uint32_t  | api Version Information                                       | Big Endian |
|                                                    | 9-63       | 56               |           | Reserved                                                      |            |
|                                                    | 64         | 8                | quint64   | Number of Data Packets in Current File                        | Big Endian |
|                                                    | 72         | 10M=10*1024*1024 | QList     | Packet Index                                                  | Big Endian |
| Configuration Information<br>msgpack<br>Byte Array | 72+10M     | 2                | uint16_t  | Configuration Information + Trace Information Length (length) | Big Endian |
|                                                    | 74+10M     |                  | double    | CenterFreq_Hz                                                 |            |
|                                                    |            |                  | double    | RefLevel_dBm                                                  |            |
|                                                    |            |                  | double    | RBW_Hz                                                        |            |
|                                                    |            |                  | double    | VBW_Hz                                                        |            |
|                                                    |            |                  | int       | RBWMode                                                       |            |
|                                                    |            |                  | int       | VBWMode                                                       |            |

|  | Byte Index | Byte Count | Data Type | Field Name              | Endianness |
|--|------------|------------|-----------|-------------------------|------------|
|  |            |            | uint32_t  | DecimateFactor          |            |
|  |            |            | int       | Window                  |            |
|  |            |            | int       | SweepTimeMode           |            |
|  |            |            | double    | SweepTime               |            |
|  |            |            | int       | Detector                |            |
|  |            |            | int       | TraceDetectMode         |            |
|  |            |            | uint32_t  | TraceDetectRatio        |            |
|  |            |            | int       | TraceDetector           |            |
|  |            |            | int       | RxPort                  |            |
|  |            |            | uint32_t  | BusTimeout_ms           |            |
|  |            |            | int       | TriggerSource           |            |
|  |            |            | int       | TriggerEdge             |            |
|  |            |            | int       | TriggerMode             |            |
|  |            |            | double    | TriggerAcqTime          |            |
|  |            |            | int       | TriggerOutMode          |            |
|  |            |            | int       | TriggerOutPulsePolarity |            |
|  |            |            | double    | TriggerLevel_dBm        |            |
|  |            |            | double    | TriggerLevel_SafeTime   |            |
|  |            |            | double    | TriggerDelay            |            |
|  |            |            | double    | PreTriggerTime          |            |
|  |            |            | int       | TriggerTimerSync        |            |
|  |            |            | double    | TriggerTimer_Period     |            |
|  |            |            | uint8_t   | EnableReTrigger         |            |
|  |            |            | double    | ReTrigger_Period        |            |
|  |            |            | uint16_t  | ReTrigger_Count         |            |
|  |            |            | int       | GainStrategy            |            |
|  |            |            | int       | Preamplifier            |            |
|  |            |            | uint8_t   | AnalogIFBWGrade         |            |
|  |            |            | uint8_t   | IFGainGrade             |            |
|  |            |            | uint8_t   | EnableDebugMode         |            |

|                                            | Byte Index | Byte Count | Data Type | Field Name                   | Endianness |
|--------------------------------------------|------------|------------|-----------|------------------------------|------------|
|                                            |            |            | int       | ReferenceClockSource         |            |
|                                            |            |            | double    | ReferenceClockFrequency      |            |
|                                            |            |            | uint8_t   | EnableReferenceClockOut      |            |
|                                            |            |            | int       | SystemClockSource            |            |
|                                            |            |            | double    | ExternalSystemClockFrequency |            |
|                                            |            |            | int8_t    | Atten                        |            |
|                                            |            |            | int       | DCCancelerMode               |            |
|                                            |            |            | int       | QDCMode                      |            |
|                                            |            |            | float     | QDCIGain                     |            |
|                                            |            |            | float     | QDCQGain                     |            |
|                                            |            |            | float     | QDCPhaseComp                 |            |
|                                            |            |            | int8_t    | DCCIOffset                   |            |
|                                            |            |            | int8_t    | DCCQOffset                   |            |
|                                            |            |            | int       | LOOptimization               |            |
| Trace Information<br>msgpack<br>Byte Array |            |            | double    | StartFrequency_Hz            |            |
|                                            |            |            | double    | StopFrequency_Hz             |            |
|                                            |            |            | double    | POI                          |            |
|                                            |            |            | double    | TraceTimestampStep           |            |
|                                            |            |            | double    | TimeResolution               |            |
|                                            |            |            | double    | PacketAcqTime                |            |
|                                            |            |            | uint32_t  | PacketCount                  |            |
|                                            |            |            | uint32_t  | PacketFrame                  |            |
|                                            |            |            | uint32_t  | FFTSize                      |            |
|                                            |            |            | uint32_t  | FrameWidth                   |            |
|                                            |            |            | uint32_t  | FrameHeight                  |            |
|                                            |            |            | uint32_t  | PacketSamplePoints           |            |
|                                            |            |            | uint32_t  | PacketValidPoints            |            |
|                                            |            |            | uint32_t  | MaxDensityValue              |            |
|                                            |            |            | uint32_t  | GainParameter                |            |

|                                                                                   | Byte Index                     | Byte Count | Data Type  | Field Name                        | Endianness         |
|-----------------------------------------------------------------------------------|--------------------------------|------------|------------|-----------------------------------|--------------------|
| Data Packet                                                                       | 74+10M+ <a href="#">length</a> | 4          | int        | Data Packet Length                | Big Endian         |
|                                                                                   |                                | N          | uint8_t *N | SpectrumStream Array              | Platform Dependent |
|                                                                                   |                                | 4          | float      | ScaleTodBm                        | Big Endian         |
|                                                                                   |                                | 4          | float      | OffsetTodBm                       | Big Endian         |
|                                                                                   |                                | 8          | uint64_t   | SpectrumBitmapIndex               | Big Endian         |
|                                                                                   |                                | 8          | uint64_t   | SysTimerCountOfFirstDataPoint     | Big Endian         |
|                                                                                   |                                | 2          | uint16_t   | InPacketTriggeredDataSize         | Big Endian         |
|                                                                                   |                                | 2          | uint16_t   | InPacketTriggerEdges              | Big Endian         |
|                                                                                   |                                | 4*25       | uint32_t   | StartDataIndexOfTriggerEdges [25] | Platform Dependent |
|                                                                                   |                                | 8*25       | uint64_t   | SysTimerCountOfEdges [25]         | Platform Dependent |
|                                                                                   |                                | 25         | int8_t     | EdgeType [25]                     | Platform Dependent |
|                                                                                   |                                | 4          | uint32_t   | MaxIndex                          | Big Endian         |
|                                                                                   |                                | 4          | float      | MaxPower_dBm                      | Big Endian         |
|                                                                                   |                                | 2          | int16_t    | Temperature                       | Big Endian         |
|                                                                                   |                                | 2          | uint16_t   | RFState                           | Big Endian         |
|                                                                                   |                                | 2          | uint16_t   | BBState                           | Big Endian         |
|                                                                                   |                                | 2          | uint16_t   | GainPattern                       | Big Endian         |
|                                                                                   |                                | 4          | uint32_t   | ConvertPattern                    | Big Endian         |
|                                                                                   |                                | 8          | double     | SysTimeStamp                      | Big Endian         |
|                                                                                   |                                | 8          | double     | AbsoluteTimeStamp                 | Big Endian         |
|                                                                                   |                                | 4          | float      | Latitude                          | Big Endian         |
|                                                                                   |                                | 4          | float      | Longitude                         | Big Endian         |
| Next Data Packet<br>(The total number of packets can be found in the File Header) |                                | 4          | int        | Data Packet Length                | Big Endian         |
|                                                                                   |                                |            |            | ...                               |                    |